

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K13764 Temperature: 24.0 °C

Model: KICHER PR Humidity: 55%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

378.5 mv/5000g

(75.7 μ v/g)

R²: 0.999910 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt

Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Operator: William Johnson

Signed

Calibration valid 2 years

From: 10Sep2024

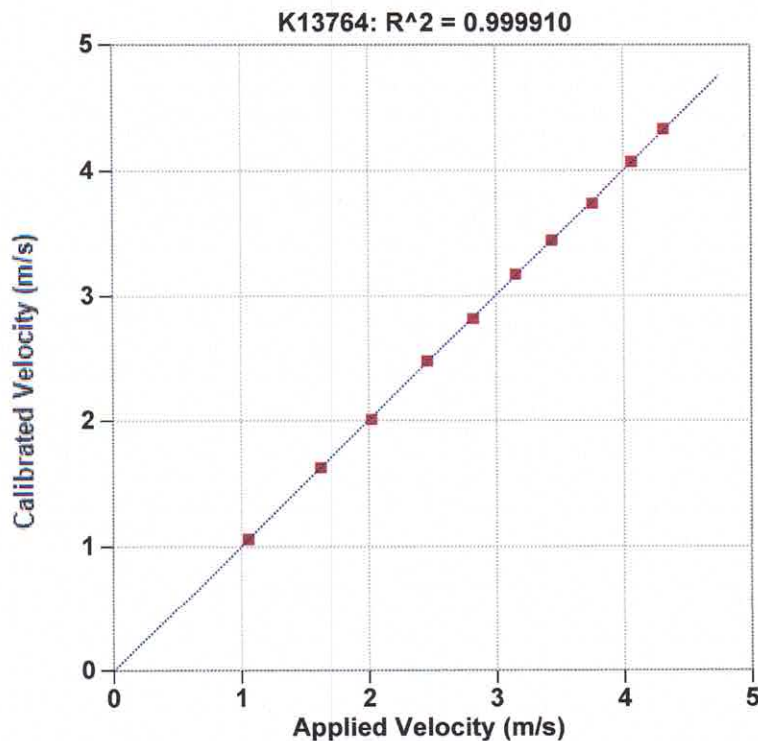

Reference Velocity	S/N K13764 Velocity
m/s	m/s
1.059	1.060
1.627	1.626
2.025	2.012
2.465	2.476
2.826	2.817
3.160	3.173
3.444	3.444
3.763	3.745
4.069	4.072
4.320	4.329

Maximum Acceleration: 941 g's