

Certificate of Calibration  
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K14135      Temperature: 24.9 °C  
Model: KICHER PR      Humidity: 48%  
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

336.3 mv/5000g  
(67.3 μv/g)  
R^2: 0.999970 [Chip programmed]


Ref Acc 1: 78270!      Cal on: 11Jan2024  
971 g's/volt  
Ref Acc 2: 78268!      Cal on: 11Jan2024  
986 g's/volt

Operator: William Johnson

  
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years  
SEP 17 2024  
From: \_\_\_\_\_

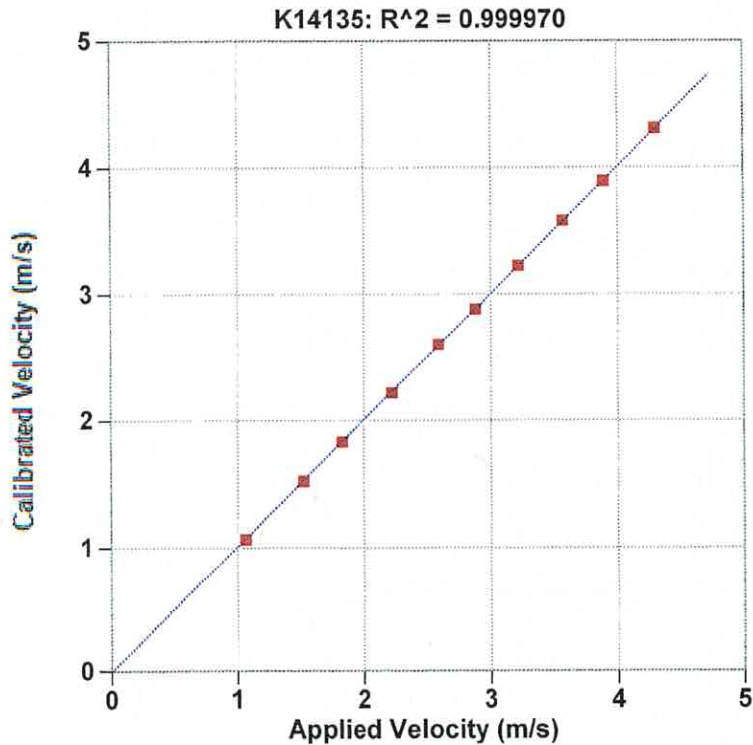

| Reference Velocity | S/N K14135 Velocity |
|--------------------|---------------------|
| m/s                | m/s                 |
| 1.067              | 1.067               |
| 1.523              | 1.518               |
| 1.830              | 1.827               |
| 2.230              | 2.217               |
| 2.591              | 2.598               |
| 2.880              | 2.881               |
| 3.227              | 3.227               |
| 3.575              | 3.578               |
| 3.895              | 3.892               |
| 4.300              | 4.305               |

Maximum Acceleration: 925 g's

