

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K14139 Temperature: 24.9 °C
Model: KICHER PR Humidity: 49%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

343.7 mv/5000g
(68.7 μ v/g)
R²: 0.999955 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: **SEP 05 2024**

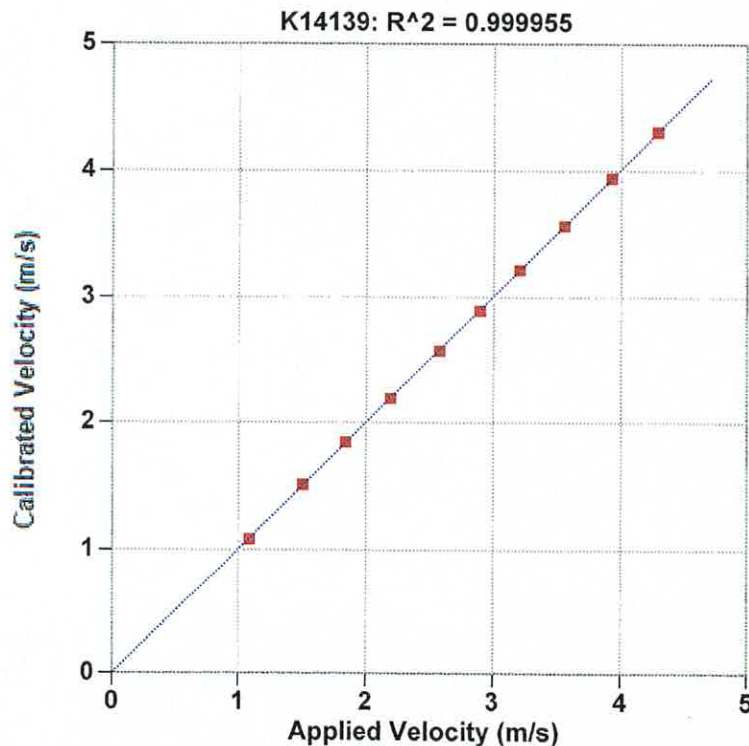

Reference Velocity	S/N K14139 Velocity
m/s	m/s
1.087	1.082
1.500	1.508
1.837	1.843
2.198	2.191
2.581	2.568
2.897	2.890
3.210	3.216
3.561	3.563
3.932	3.938
4.295	4.297

Maximum Acceleration: 923 g's

