

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: LW196275 Temperature: 21.8 °C
Model: PE Humidity: 50%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

9.8 g's/volt
R^2: 0.999960 [No chip]

Ref Acc 1: LW503313! Cal on: 31Jan2024
10 g's/volt
Ref Acc 2: LW503311! Cal on: 31Jan2024
10 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 10Sep2024

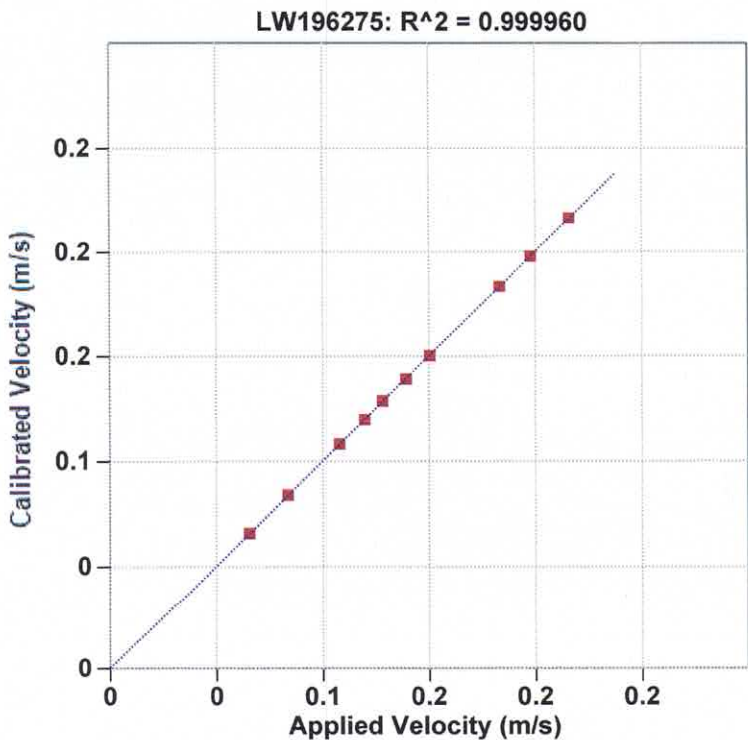

Reference Velocity	S/N LW196275 Velocity
m/s	m/s
0.066	0.066
0.084	0.084
0.108	0.108
0.120	0.120
0.128	0.129
0.139	0.139
0.151	0.150
0.183	0.184
0.198	0.198
0.216	0.216

Maximum Acceleration: 23 g's