


Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

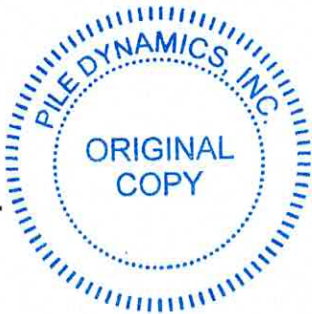

Serial No: LW503307 Temperature: 23.8 °C
Model: PE Humidity: 52%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

9.9 g's/volt

R^2: 0.999954 [Chip programmed]

Ref Acc 1: LW503311! Cal on: 31Jan2024
10 g's/volt
Ref Acc 2: LW503313! Cal on: 31Jan2024
10 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: SEP 13 2024

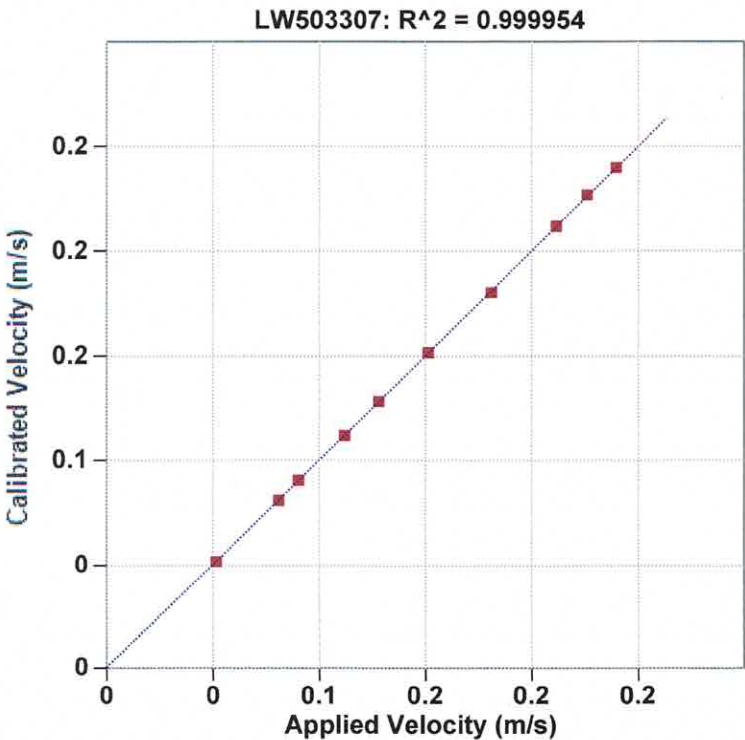

Reference Velocity	S/N LW503307 Velocity
m/s	m/s
0.052	0.052
0.081	0.081
0.090	0.090
0.112	0.112
0.128	0.128
0.151	0.152
0.181	0.180
0.212	0.212
0.226	0.227
0.240	0.240
Maximum Acceleration: 26 g's	