Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: N802
PDI Gage Factor: 143.4
Mean Linear Correlation Coefficient: 0.999725

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1883.2	-3.900	308.4	0.625
-1456.7	-3.022	695.5	1.389
-1082.7	-2.218	1069.6	2.117
-721.8	-1.476	1430.4	2.827
-413.4	-0.838	1797.9	3.535
-98.4	-0.175	1988.2	3.908

Calibration Curve

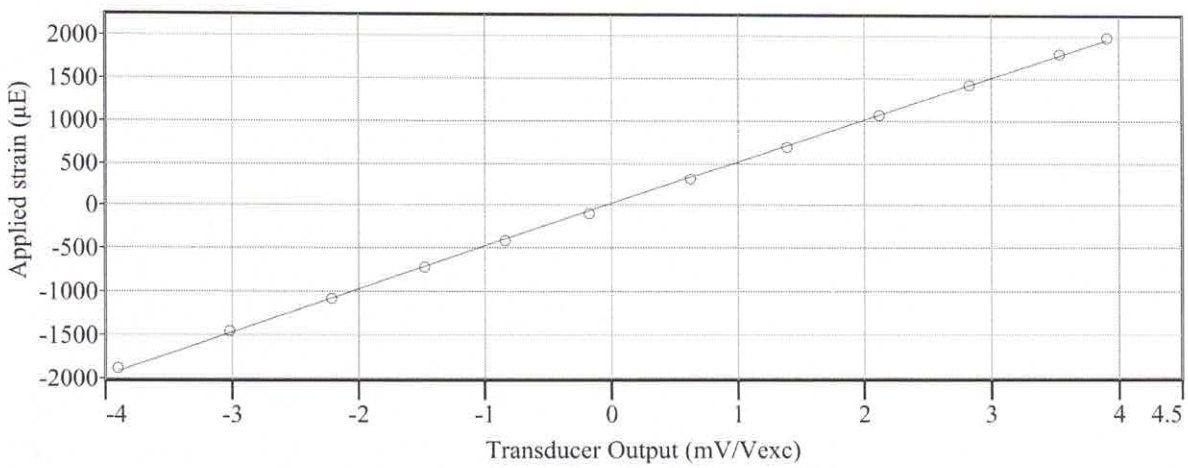

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: N802
Calibration Date: 9/20/2024 6:18:51 AM