Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: U490
PDI Gage Factor: 141.7
Mean Linear Correlation Coefficient: 0.999903

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-2126.0	-4.401	282.2	0.582
-1758.5	-3.616	649.6	1.326
-1351.7	-2.789	1003.9	2.033
-925.2	-1.900	1364.8	2.749
-531.5	-1.075	1719.2	3.471
-111.5	-0.211	1994.8	4.000

Calibration Curve

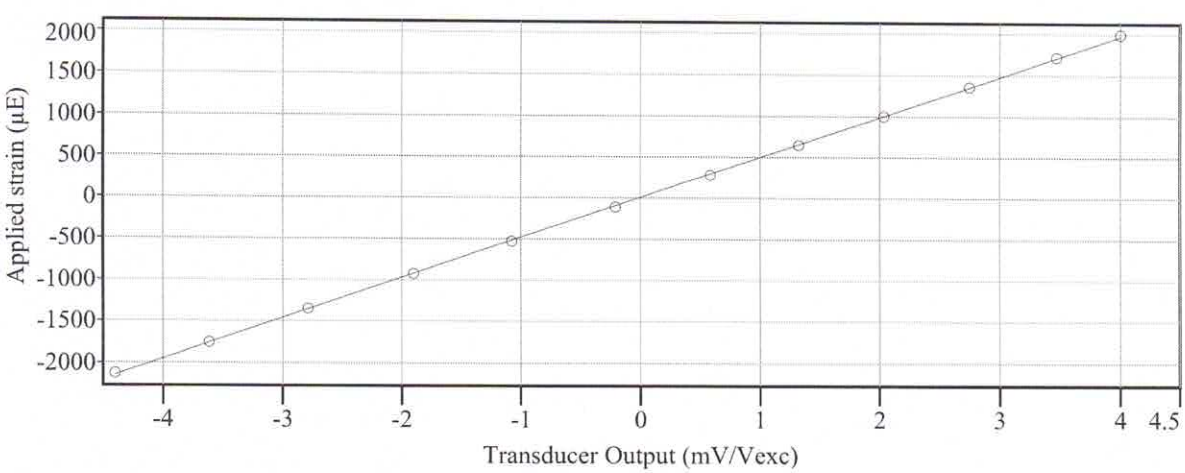

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: U490
Calibration Date: 9/20/2024 6:22:48 AM

Pile Dynamics, Inc.