Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: Z393
PDI Gage Factor: 95.6
Mean Linear Correlation Coefficient: 0.999931

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2185.0	-6.557	315.0	1.009
-1660.1	-5.008	728.3	2.267
-1161.4	-3.474	1115.5	3.480
-691.2	-2.050	1489.5	4.574
-374.0	-1.075	1824.1	5.540
-39.4	-0.079	1955.4	5.880

Calibration Curve

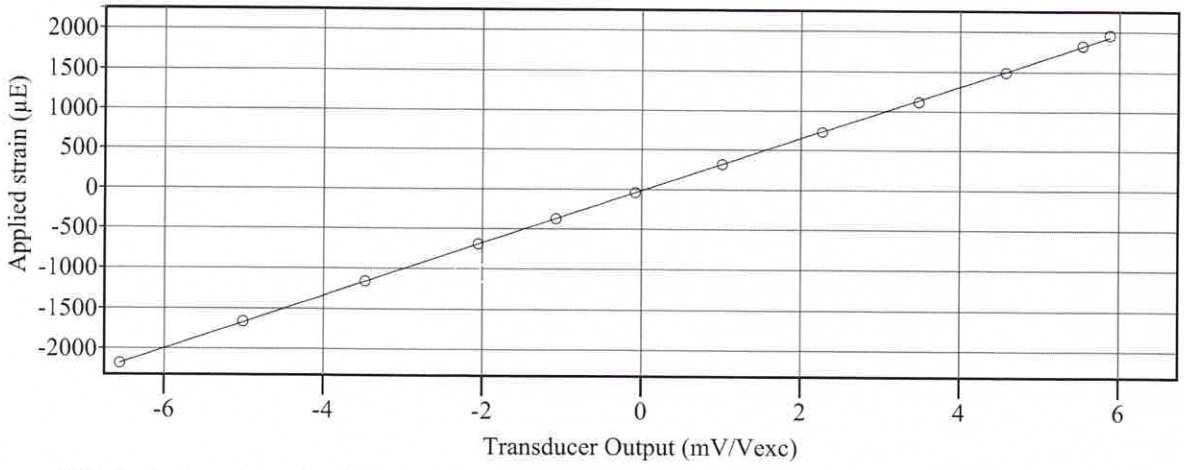

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: Z393
Calibration Date: SEP 2 5 2024

Pile Dynamics, Inc.