Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: Z397
PDI Gage Factor: 93.5
Mean Linear Correlation Coefficient: 0.999940

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-2139.1	-6.573	347.8	1.157
-1638.2	-5.010	761.2	2.450
-1128.6	-3.464	1187.7	3.740
-684.6	-2.056	1561.7	4.880
-367.5	-1.073	1948.8	6.002
-26.2	-0.030		

Calibration Curve

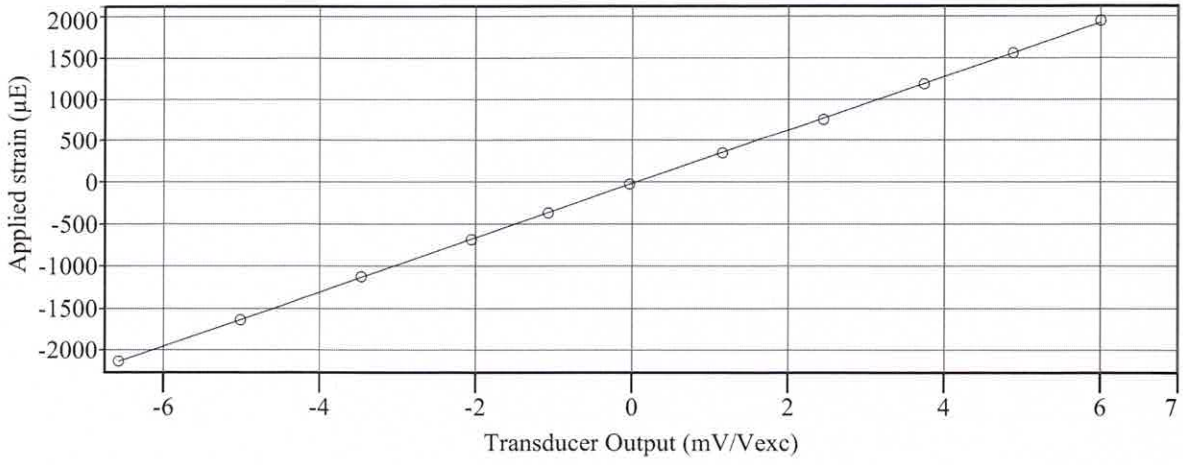

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: Z397
Calibration Date: JUL 19 2024

Pile Dynamics, Inc.