Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: Z667
PDI Gage Factor: 97.3
Mean Linear Correlation Coefficient: 0.999884

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2066.9	-6.127	446.2	1.425
-1555.1	-4.576	872.7	2.685
-1069.6	-3.125	1200.8	3.669
-616.8	-1.773	1515.7	4.583
-249.3	-0.678	1843.8	5.483
78.7	0.309	2053.8	6.057

Calibration Curve

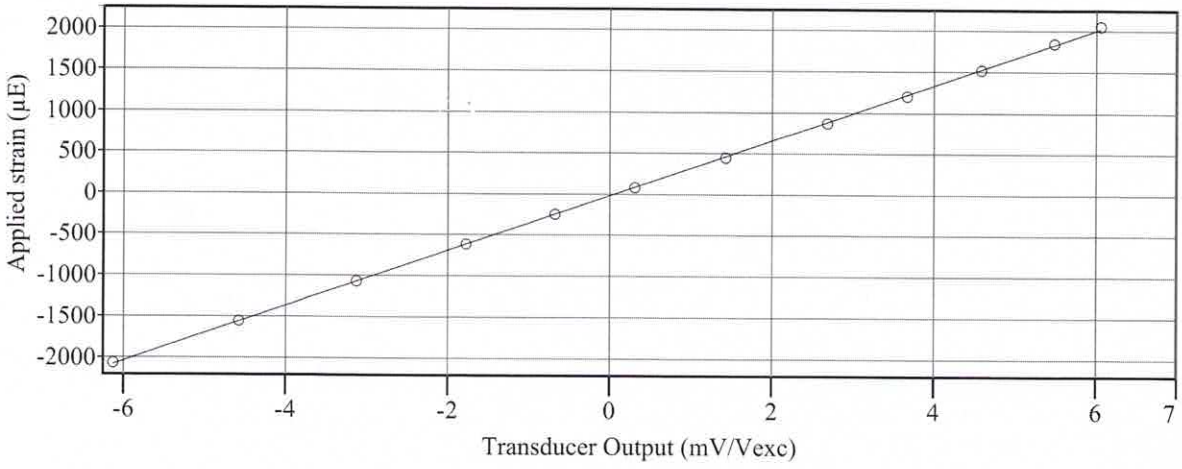

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: Z667
Calibration Date: SEP 2 7 2024

Pile Dynamics, Inc.