Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: Z669
PDI Gage Factor: 95.9
Mean Linear Correlation Coefficient: 0.999903

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1988.2	-5.961	452.8	1.470
-1489.5	-4.439	820.2	2.585
-1017.1	-3.024	1141.7	3.539
-584.0	-1.708	1465.4	4.490
-262.5	-0.720	1791.3	5.418
65.6	0.275	2001.3	6.011

Calibration Curve

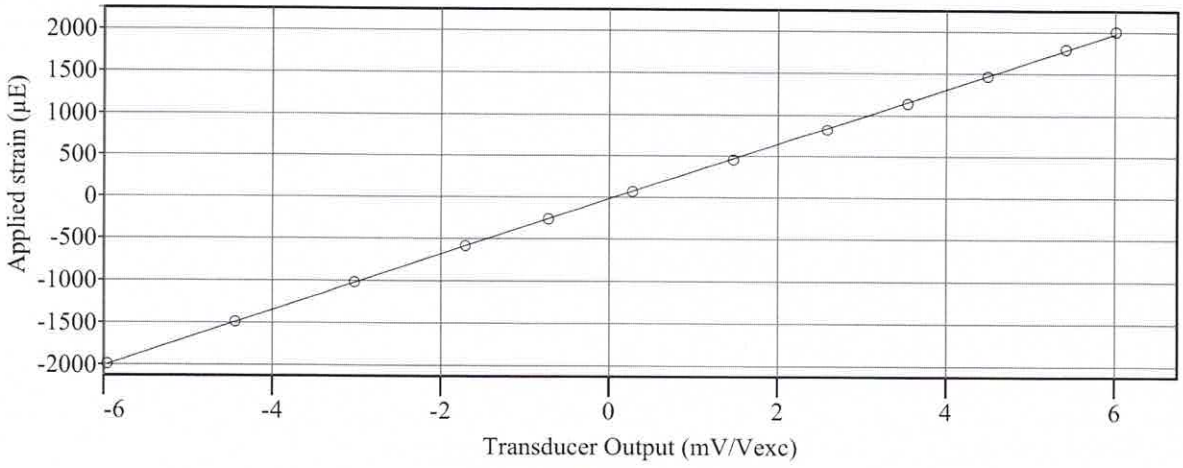

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: Z669
Calibration Date: SEP 2 7 2024

Pile Dynamics, Inc.