Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: G722
PDI Gage Factor: 92.0
Mean Linear Correlation Coefficient: 0.999869

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-2139.1	-6.630	255.9	0.977
-1607.6	-4.952	610.2	2.090
-1128.6	-3.458	990.8	3.273
-748.0	-2.250	1391.1	4.510
-393.7	-1.119	1771.7	5.643
-78.7	-0.078	1994.8	6.283

Calibration Curve

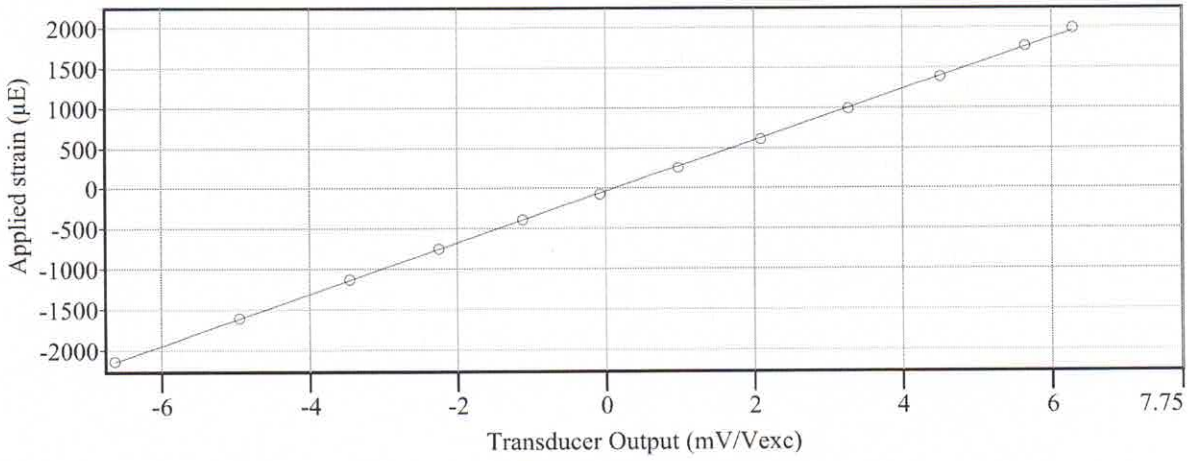

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman Signature: Paul Hartman

PDI Gage: G722
Calibration Date: 9/25/2024 12:48:09 PM

Pile Dynamics, Inc.