Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K11184	**Temperature:**	23.6 °C
Model:	KICHER PR	**Humidity:**	44%
Calibrated on:	Channel 4 on 8G 5161 LE		

Ref Acc 1:	78270! 971 g's/volt	**Cal on:**	11Jan2024
Ref Acc 2:	78268! 986 g's/volt	**Cal on:**	11Jan2024

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

373.4 mv/5000g
(74.7 µv/g)
R^2: 0.999951 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: 25Sep2024

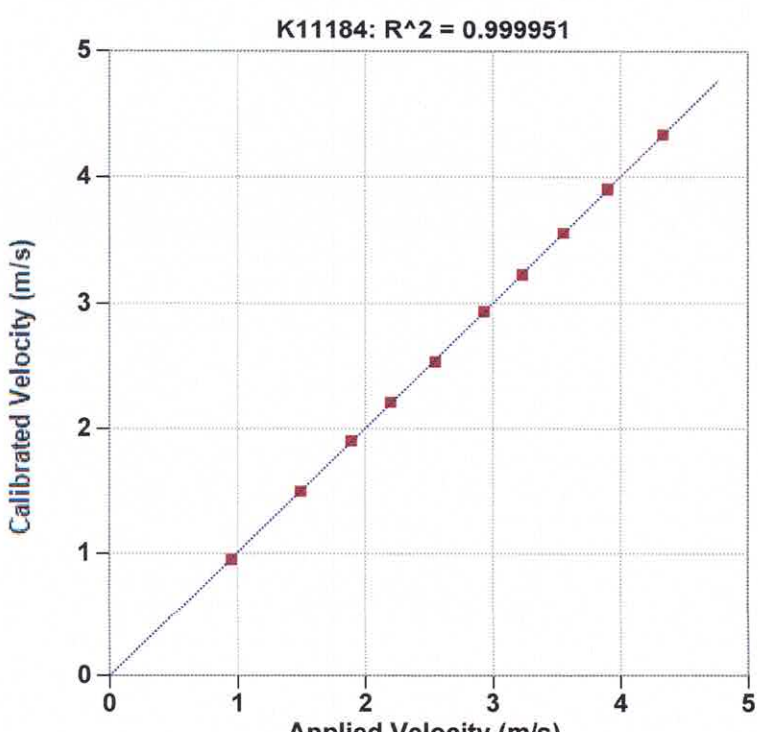

Reference Velocity	S/N K11184 Velocity
m/s	m/s
0.958	0.953
1.499	1.500
1.896	1.905
2.205	2.214
2.553	2.537
2.935	2.936
3.235	3.227
3.556	3.560
3.903	3.906
4.339	4.341

Maximum Acceleration: 945 g's