Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

Serial No:	K11425	**Temperature:**	23.6 °C
Model:	KICHER PR	**Humidity:**	44%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	78270! 971 g's/volt	**Cal on:**	11Jan2024
Ref Acc 2:	78268! 986 g's/volt	**Cal on:**	11Jan2024

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

287.7 mv/5000g
(57.5 µv/g)
R^2: 0.999963 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: 25Sep2024

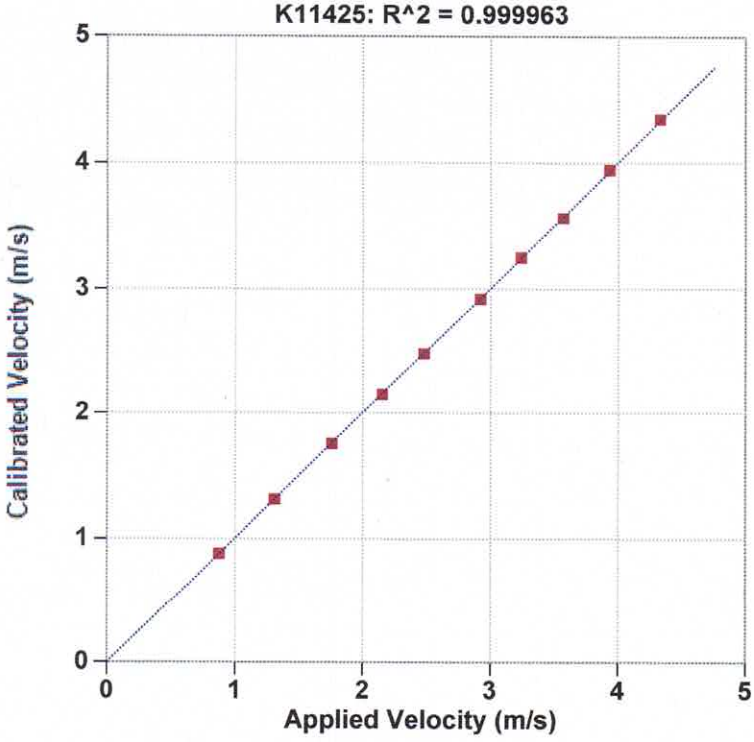

Reference Velocity	S/N K11425 Velocity
m/s	m/s
0.878	0.883
1.315	1.313
1.762	1.756
2.157	2.149
2.485	2.480
2.924	2.919
3.244	3.249
3.574	3.565
3.938	3.946
4.334	4.344

Maximum Acceleration: 944 g's