Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

PILE DYNAMICS, INC. ORIGINAL COPY

Serial No:	K14258	**Temperature:**	23.3 °C
Model:	KICHER PR	**Humidity:**	32%
Calibrated on:	Channel 3 on 8G 5161 LE		

Ref Acc 1:	78268! 986 g's/volt	**Cal on:**	11Jan2024
Ref Acc 2:	78270! 971 g's/volt	**Cal on:**	11Jan2024

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

361.8 mv/5000g
(72.4 µv/g)
R^2: 0.999955 [Chip programmed]

Operator: William Johnson

Signed

Calibration valid 2 years

From: OCT 2 5 2024

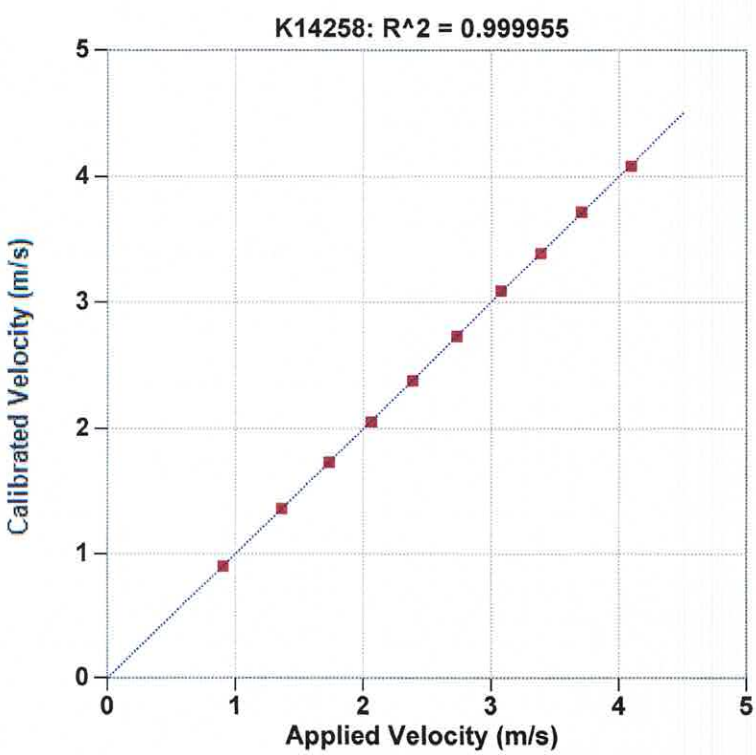

Reference Velocity	S/N K14258 Velocity
m/s	m/s
0.906	0.905
1.364	1.366
1.735	1.733
2.066	2.059
2.388	2.384
2.734	2.733
3.079	3.090
3.390	3.389
3.707	3.718
4.096	4.085

Maximum Acceleration: 889 g's