Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: P129
PDI Gage Factor: 92.1
Mean Linear Correlation Coefficient: 0.999590

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-1953.2	-6.313	315.0	1.032
-1528.9	-4.904	721.8	2.283
-1128.6	-3.609	1108.9	3.462
-774.3	-2.433	1489.5	4.612
-452.8	-1.387	1876.6	5.734
-105.0	-0.292	1996.9	6.093

Calibration Curve

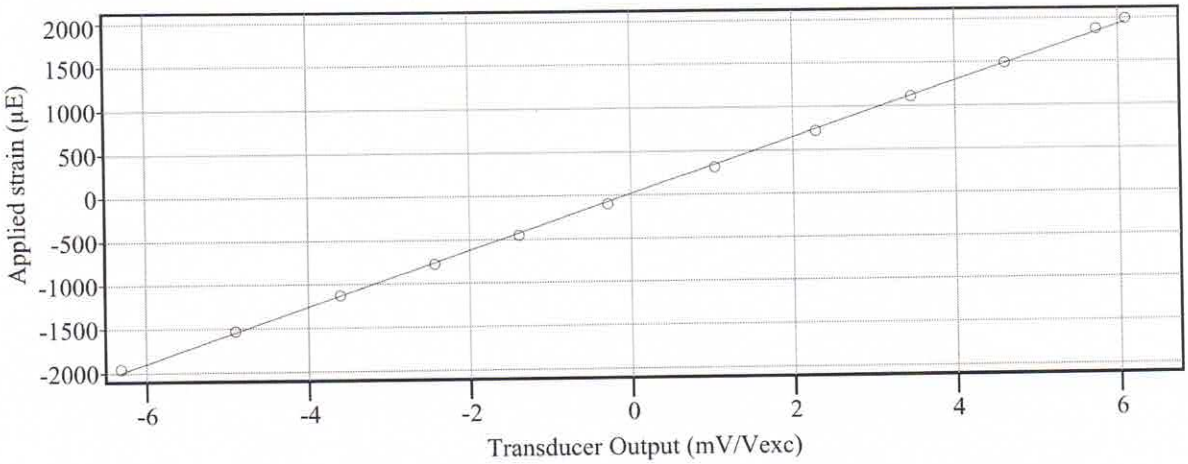

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: P129
Calibration Date: 9/26/2024 12:53:22 PM

Pile Dynamics, Inc.