




# Certificate of Calibration

Pile Dynamics, Inc.  
 Transducer Model: PDI Strain Transducer  
 Serial Number: C213  
 PDI Gage Factor: 91.0  
 Mean Linear Correlation Coefficient: 0.999578

Table 1: Representative Calibration Data

Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)
-2034.1	-6.516	590.6	1.927
-1482.9	-4.827	866.1	2.774
-999.6	-3.297	1135.2	3.577
-616.8	-2.052	1395.5	4.356
-306.2	-0.966	1640.4	5.095
-13.1	0.022	1918.2	5.920
282.2	0.963		

Calibration Curve

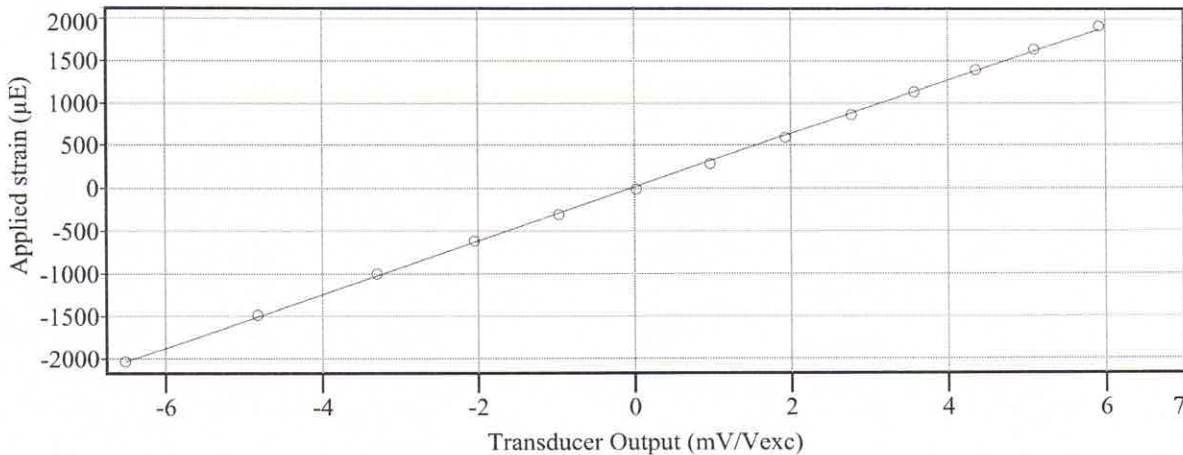

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: \_\_\_\_\_

*Paul Hartman*

PDI Gage: C213

Calibration Date: 11/18/2024 8:46:05 AM

