




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: P138
 PDI Gage Factor: 89.6
 Mean Linear Correlation Coefficient: 0.999571

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1955.4	-6.432	360.9	1.222
-1417.3	-4.729	761.2	2.453
-997.4	-3.322	1115.5	3.592
-649.6	-2.154	1476.4	4.659
-341.2	-1.074	1817.6	5.735
-26.2	-0.027	2007.9	6.279

Calibration Curve

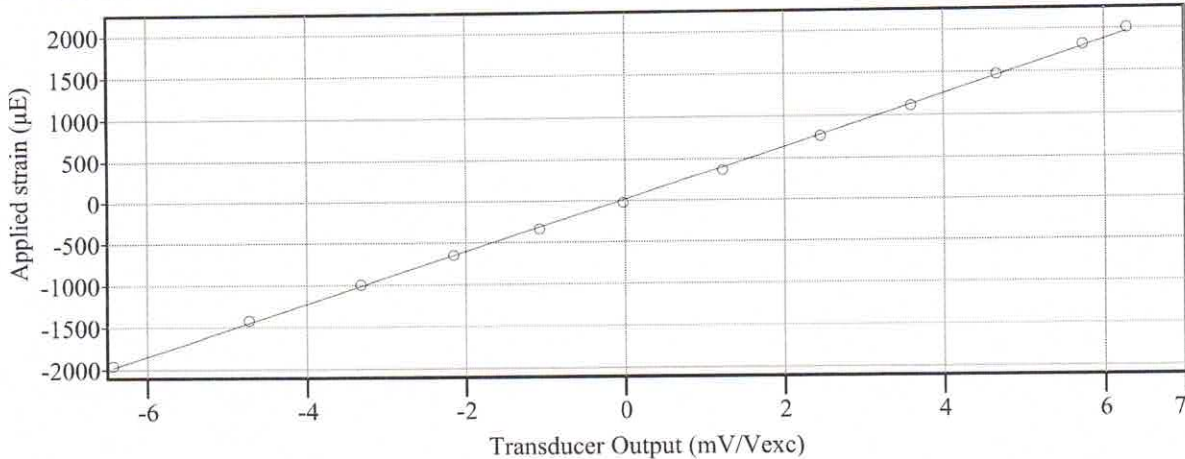

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: P138

Calibration Date: 11/18/2024 1:45:46 PM

