



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: 521A


PDI Gage Factor: 93.0

Mean Linear Correlation Coefficient: 0.999988

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1896.3	-5.766	505.2	1.694
-1404.2	-4.228	912.1	2.991
-944.9	-2.787	1286.1	4.148
-511.8	-1.448	1601.0	5.112
-164.0	-0.378	1935.7	6.124
137.8	0.580	2007.9	6.362

Calibration Curve

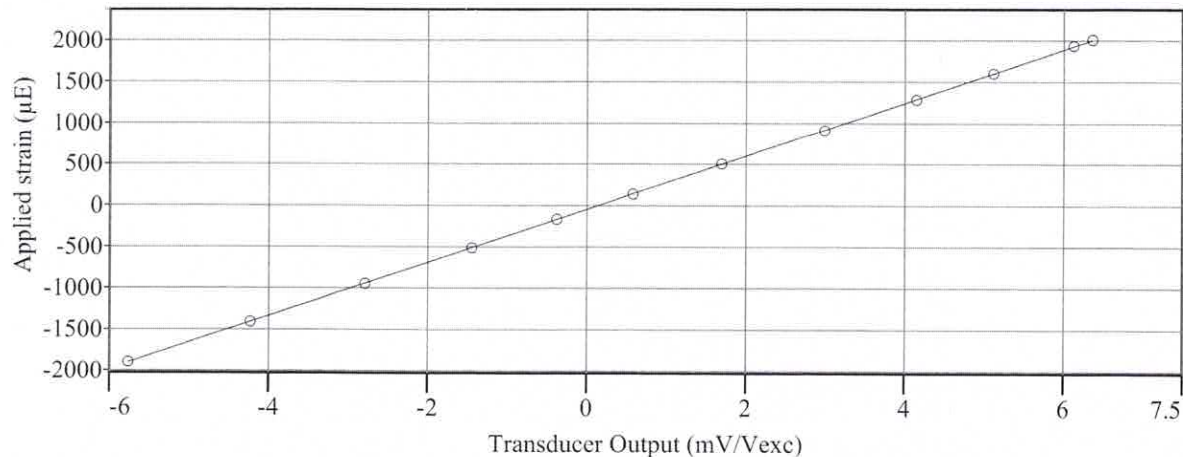

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: VANNA OUK

Signature:

PDI Gage: 521A

Calibration Date: DEC 20 2024

