




# Certificate of Calibration

Pile Dynamics, Inc.  
 Transducer Model: PDI Strain Transducer  
 Serial Number: H818  
 PDI Gage Factor: 94.6  
 Mean Linear Correlation Coefficient: 0.999733

Table 1: Representative Calibration Data

Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)
-2097.6	-6.207	214.3	1.020
-1574.8	-4.606	636.5	2.261
-1181.1	-3.360	1032.4	3.447
-807.1	-2.164	1430.4	4.616
-463.7	-1.083	1817.6	5.766
-144.4	-0.068	1988.2	6.250

Calibration Curve

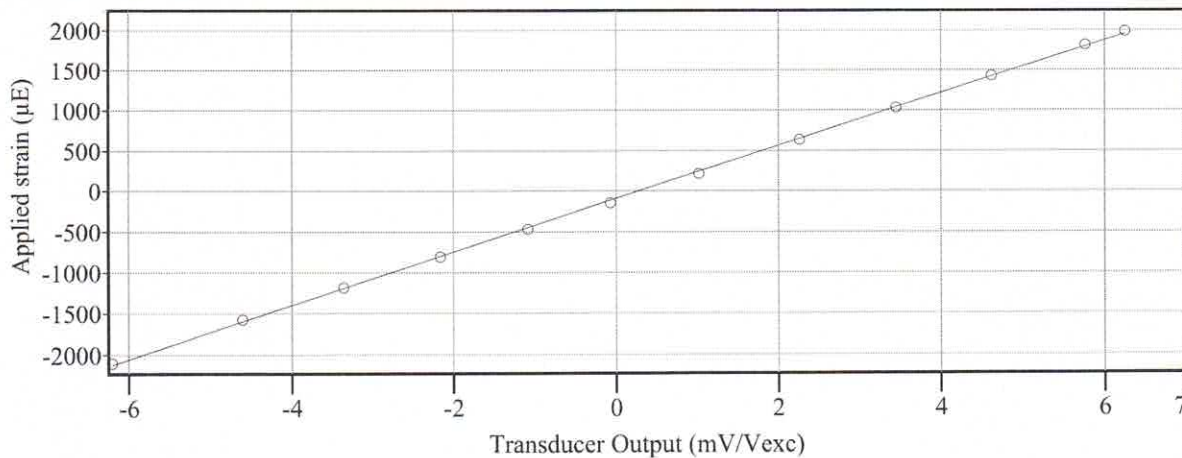


PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: 

PDI Gage: H818

Calibration Date: 1/7/2025 9:17:20 AM

