

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 60641 Temperature: 23.5 °C
Model: PE Humidity: 33%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

1236.2 g's/volt

R²: 0.999942 [No chip]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 05Mar2025

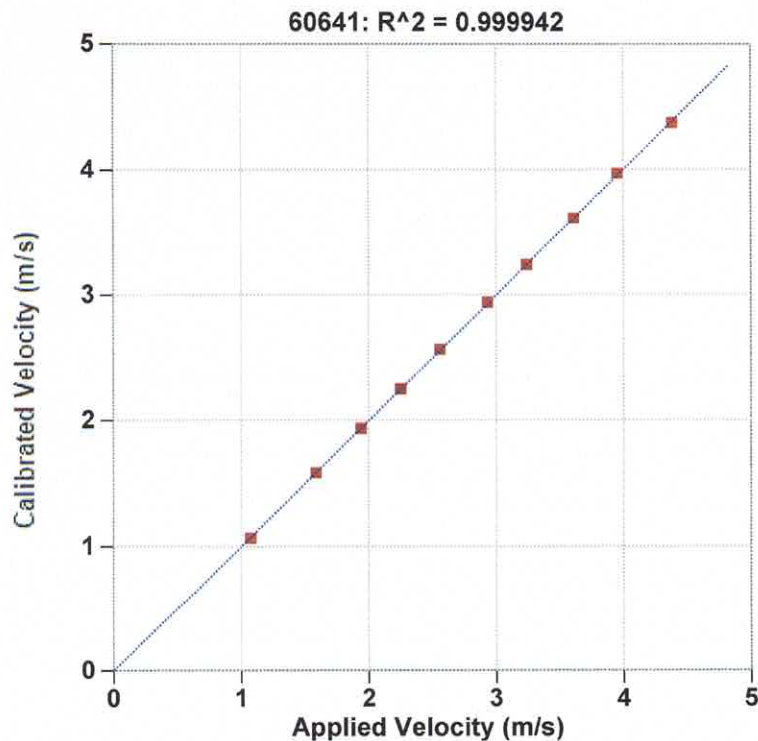

Reference Velocity	S/N 60641 Velocity
m/s	m/s
1.075	1.066
1.585	1.581
1.938	1.933
2.252	2.250
2.559	2.563
2.933	2.940
3.240	3.234
3.609	3.608
3.954	3.970
4.382	4.373

Maximum Acceleration: 967 g's