

Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 66054 Temperature: 23.5 °C
Model: PE Humidity: 33%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

1021.4 g's/volt

R²: 0.999929 [No chip]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 05Mar2025

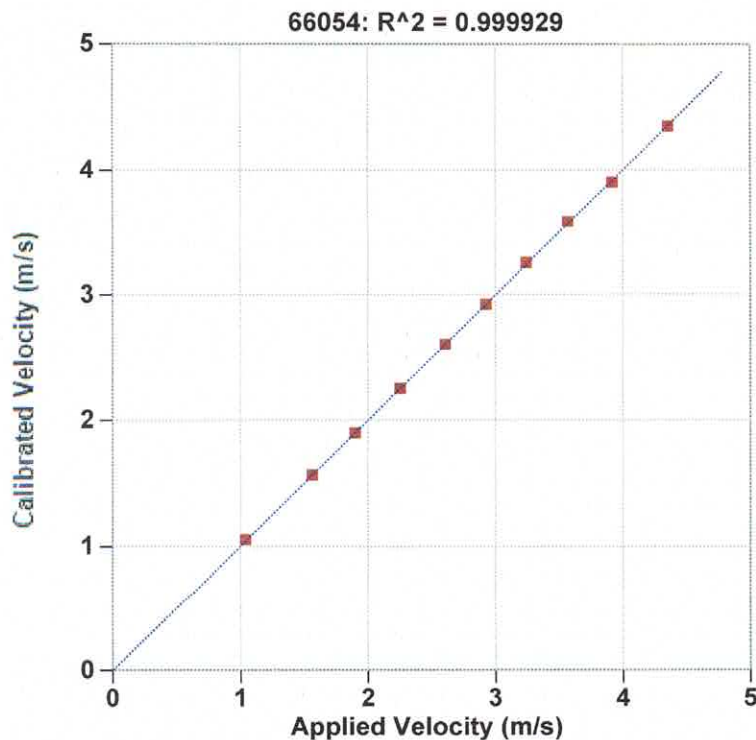

Reference Velocity	S/N 66054 Velocity
m/s	m/s
1.041	1.052
1.563	1.565
1.898	1.899
2.254	2.253
2.606	2.604
2.925	2.921
3.242	3.253
3.568	3.581
3.915	3.900
4.354	4.349
Maximum Acceleration: 960 g's	