

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K11418 Temperature: 23.5 °C
Model: KICHER PR Humidity: 25%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

394.0 mv/5000g
(78.8 μ v/g)
R²: 0.999958 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 04Mar2025

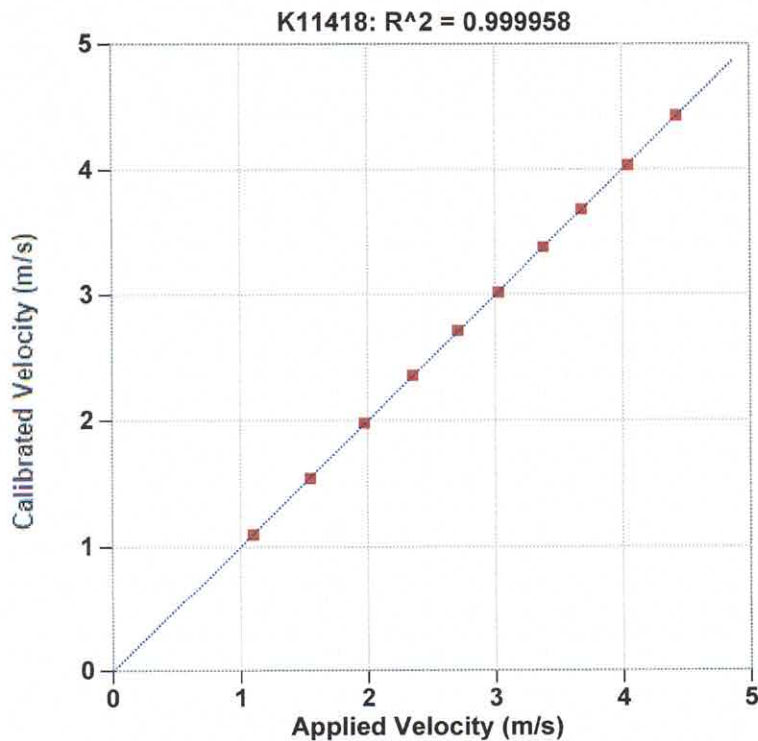

Reference Velocity	S/N K11418 Velocity
m/s	m/s
1.101	1.098
1.550	1.541
1.972	1.982
2.352	2.355
2.707	2.715
3.026	3.017
3.379	3.374
3.678	3.682
4.044	4.037
4.425	4.431

Maximum Acceleration: 977 g's