

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K12192 Temperature: 23.3 °C
Model: KICHER PR Humidity: 26%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

390.5 mv/5000g
(78.1 μ v/g)
R²: 0.999949 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 03Mar2025

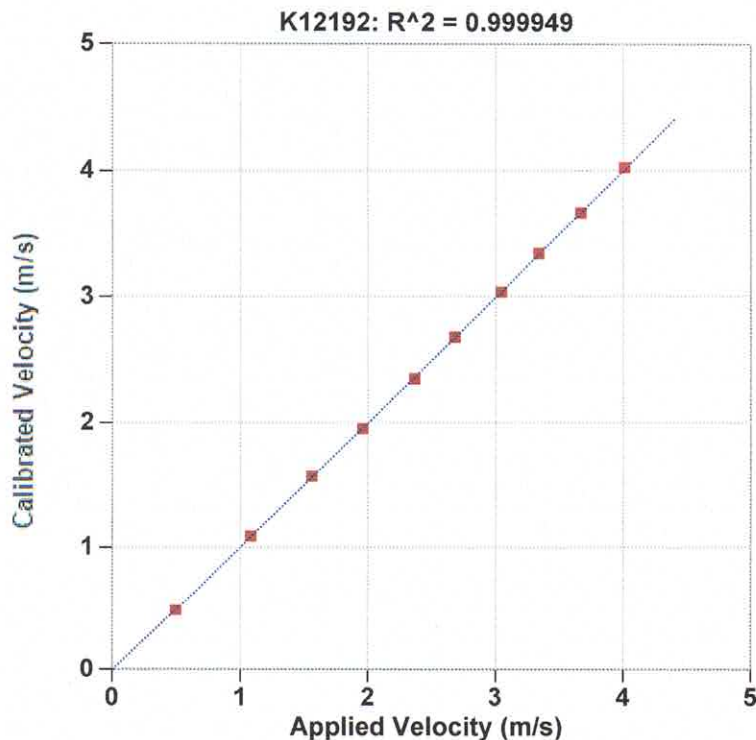

Reference Velocity	S/N K12192 Velocity
m/s	m/s
0.493	0.492
1.083	1.090
1.560	1.568
1.958	1.951
2.365	2.350
2.680	2.682
3.043	3.035
3.337	3.338
3.665	3.663
4.009	4.022

Maximum Acceleration: 877 g's