

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K12432 Temperature: 22.1 °C

Model: KICHER PR Humidity: 26%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

493.7 mv/5000g

(98.7 μ v/g)

R²: 0.999901 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt

Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: 07Mar2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

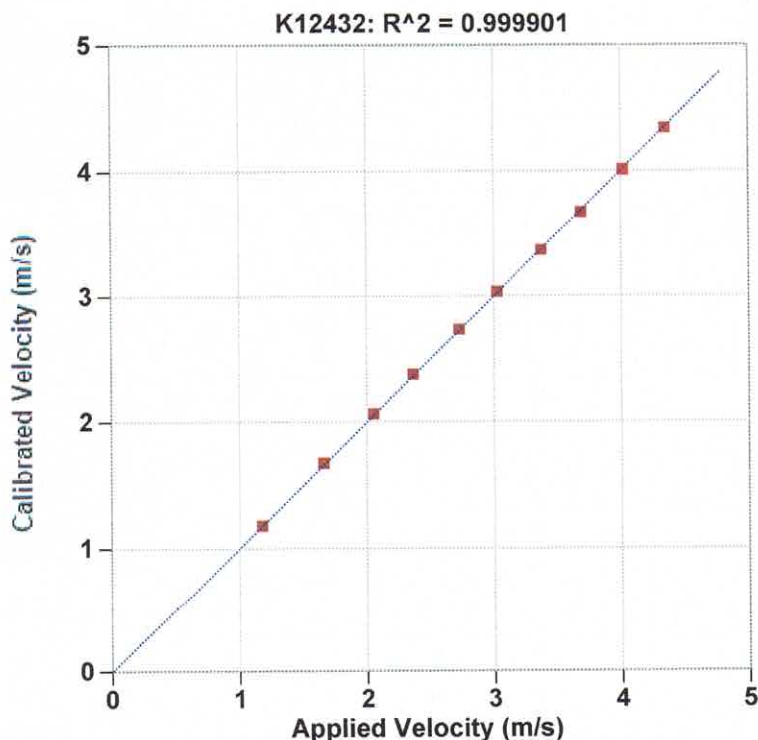

Reference Velocity	S/N K12432 Velocity
m/s	m/s
1.178	1.180
1.661	1.675
2.053	2.064
2.365	2.376
2.726	2.732
3.024	3.036
3.371	3.366
3.686	3.672
4.018	4.010
4.345	4.339
Maximum Acceleration: 960 g's	