

Certificate of Calibration  
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K3400      Temperature: 23.5 °C  
Model: KICHER PR      Humidity: 25%  
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

384.6 mv/5000g  
(76.9 μv/g)  
R^2: 0.999954 [Chip programmed]

Ref Acc 1: 78270!      Cal on: 11Jan2024  
971 g's/volt  
Ref Acc 2: 78268!      Cal on: 11Jan2024  
986 g's/volt


Operator: William Johnson

  
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 04Mar2025

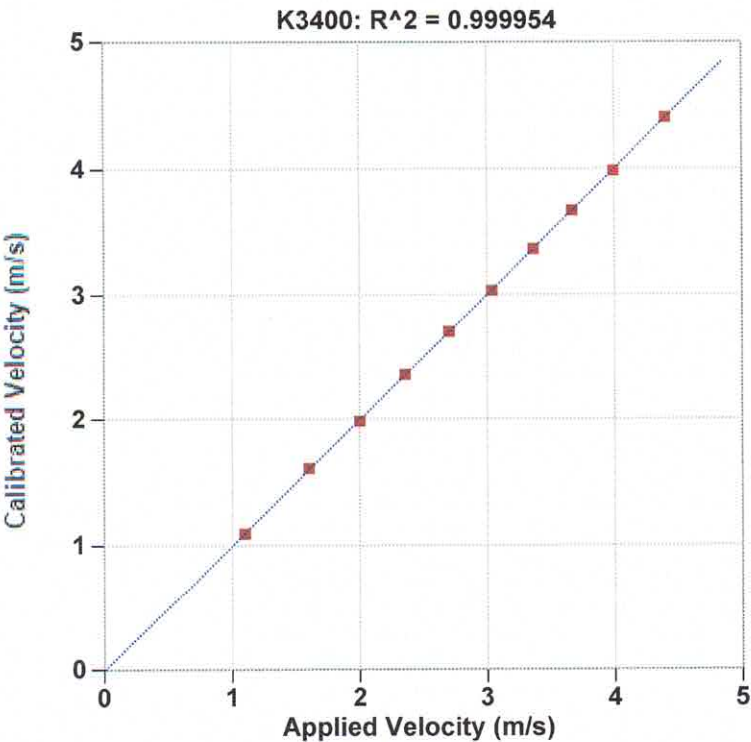

| Reference Velocity            | S/N K3400 Velocity |
|-------------------------------|--------------------|
| m/s                           | m/s                |
| 1.099                         | 1.096              |
| 1.600                         | 1.614              |
| 2.000                         | 1.988              |
| 2.358                         | 2.363              |
| 2.701                         | 2.708              |
| 3.038                         | 3.036              |
| 3.365                         | 3.365              |
| 3.668                         | 3.670              |
| 3.994                         | 3.986              |
| 4.401                         | 4.401              |
| Maximum Acceleration: 969 g's |                    |