

Certificate of Calibration  
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K3740      Temperature: 21.5 °C  
Model: KICHER PR      Humidity: 26%  
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

372.1 mv/5000g  
(74.4 μv/g)  
R^2: 0.999913 [Chip programmed]

Ref Acc 1: 78270!      Cal on: 11Jan2024  
971 g's/volt  
Ref Acc 2: 78268!      Cal on: 11Jan2024  
986 g's/volt


Operator: William Johnson

  
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 07Mar2025

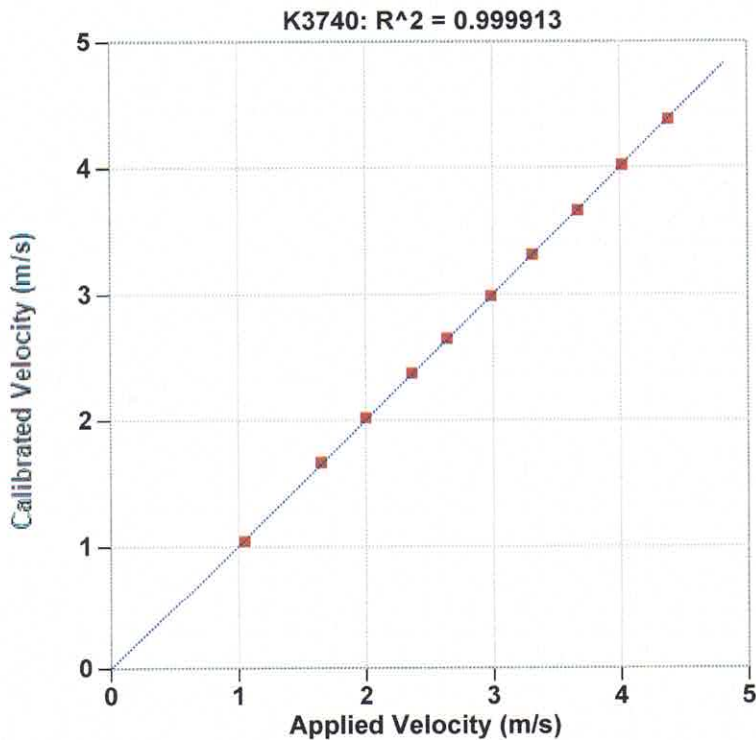

| Reference Velocity | S/N K3740 Velocity |
|--------------------|--------------------|
| m/s                | m/s                |
| 1.047              | 1.035              |
| 1.648              | 1.665              |
| 2.000              | 2.015              |
| 2.363              | 2.371              |
| 2.641              | 2.647              |
| 2.984              | 2.982              |
| 3.309              | 3.305              |
| 3.669              | 3.663              |
| 4.018              | 4.014              |
| 4.380              | 4.374              |

Maximum Acceleration: 969 g's