

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K4847 Temperature: 23.5 °C
Model: KICHER PR Humidity: 25%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

374.7 mv/5000g
(74.9 μ v/g)
R²: 0.999958 [Chip programmed]


Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt

Operator: William Johnson


Signed

Calibration valid 2 years

From: 04Mar2025

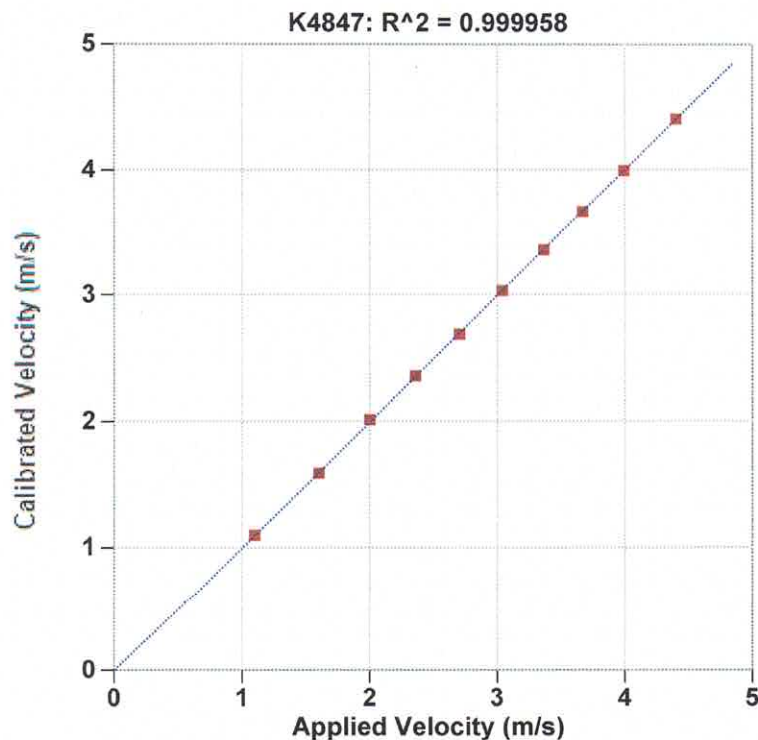

Reference Velocity	S/N K4847 Velocity
m/s	m/s
1.099	1.100
1.600	1.594
2.000	2.016
2.358	2.362
2.701	2.693
3.038	3.036
3.365	3.361
3.668	3.664
3.994	3.996
4.401	4.404

Maximum Acceleration: 969 g's