



Certificate of Calibration

TechSense

Transducer Model: PDI Strain Transducer

Serial Number: P492


PDI Gage Factor: 90.3

Mean Linear Correlation Coefficient: 0.999963

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1799.7	-6.002	548.4	1.862
-1515.2	-5.080	897.5	3.027
-1152.6	-3.846	1109.0	3.745
-834.0	-2.732	1450.3	4.890
-491.7	-1.625	1693.0	5.678
-147.1	-0.479	2135.5	7.120
199.2	0.693		

Calibration Curve

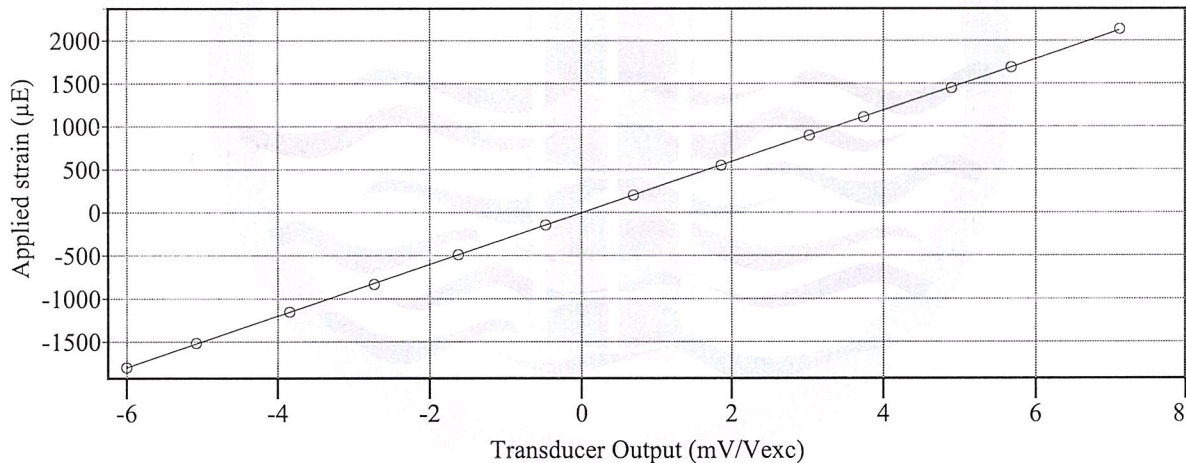

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1003HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC


PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: RASENDU PATEL

Signature: _____

PDI Gage: P492

Calibration Date: 27-09-2024 16:27:51

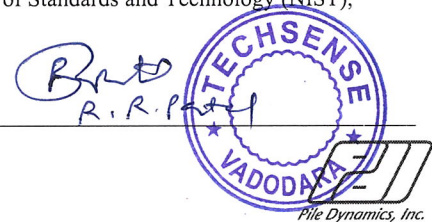

TechSense

49, Atmajyoti Nagar Society, Near Atmajyoti Ashram, Ellora Park, Vadodara - 390023

Website : www.techsenseindia.com E-mail : info@techsenseindia.com

Mobile.: +91- 8905510013 / +91 9327226069