



Certificate of Calibration

TechSense

Transducer Model: PDI Strain Transducer

Serial Number: W029


PDI Gage Factor: 92.3

Mean Linear Correlation Coefficient: 0.999626

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1669.0	-5.638	202.8	0.603
-1303.7	-4.422	487.3	1.589
-962.9	-3.323	868.0	2.791
-646.5	-2.231	1151.2	3.672
-320.1	-1.129	1561.8	4.944
-98.1	-0.385	1952.5	6.129

Calibration Curve

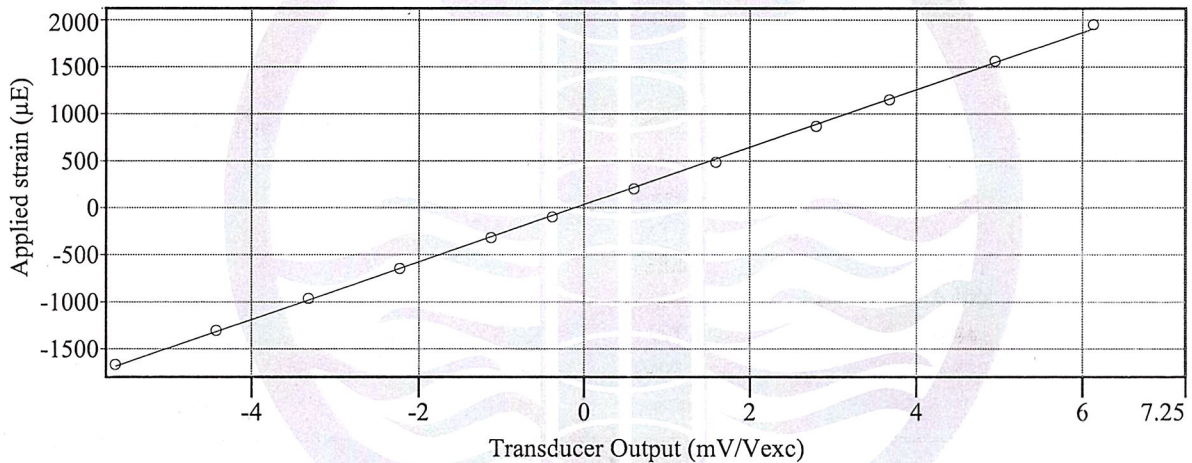

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1003HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: RASENDU PATEL

Signature: _____

PDI Gage: W029

Calibration Date: 10-01-2024 12:12:12



TechSense

49, Atmajyoti Nagar Society, Near Atmajyoti Ashram, Ellora Park, Vadodara - 390023
Website : www.techsenseindia.com E-mail : info@techsenseindia.com
Mobile.: +91- 8905510013 / +91 9327226069