




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: W216
 PDI Gage Factor: 91.2
 Mean Linear Correlation Coefficient: 0.999704

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2106.3	-6.877	282.2	1.045
-1596.7	-5.230	651.8	2.234
-1154.9	-3.784	1003.9	3.343
-759.0	-2.469	1327.6	4.332
-400.3	-1.256	1640.4	5.301
-59.1	-0.106	1975.1	6.305

Calibration Curve

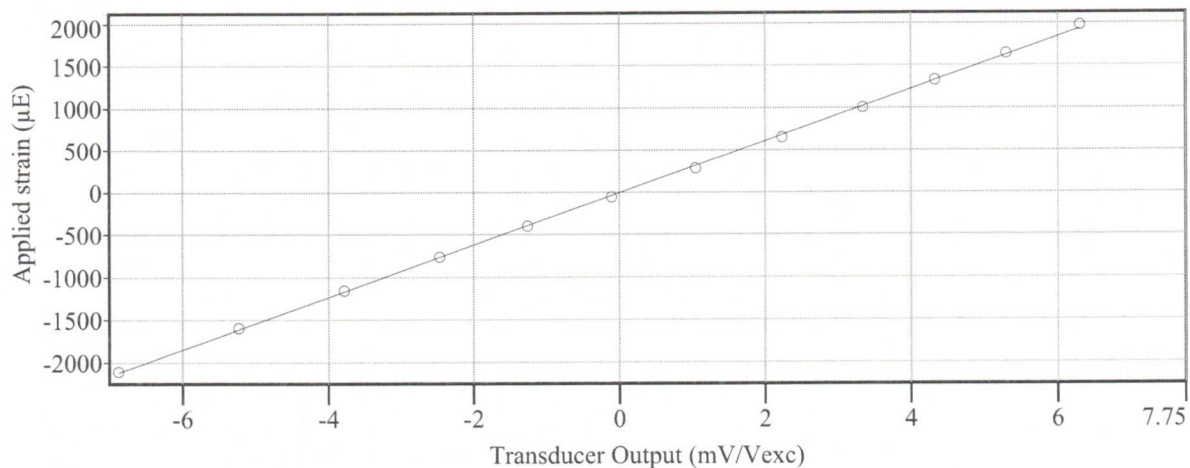

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: W216

Calibration Date: 3/10/2025 7:41:58 AM

