

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: 71205 Temperature: 22.1 °C
Model: PE Humidity: 26%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

1030.0 g's/volt

R²: 0.999981 [Chip programmed]

Ref Acc 1: 78268! Cal on: 11Jan2024
986 g's/volt
Ref Acc 2: 78270! Cal on: 11Jan2024
971 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 14Mar2025

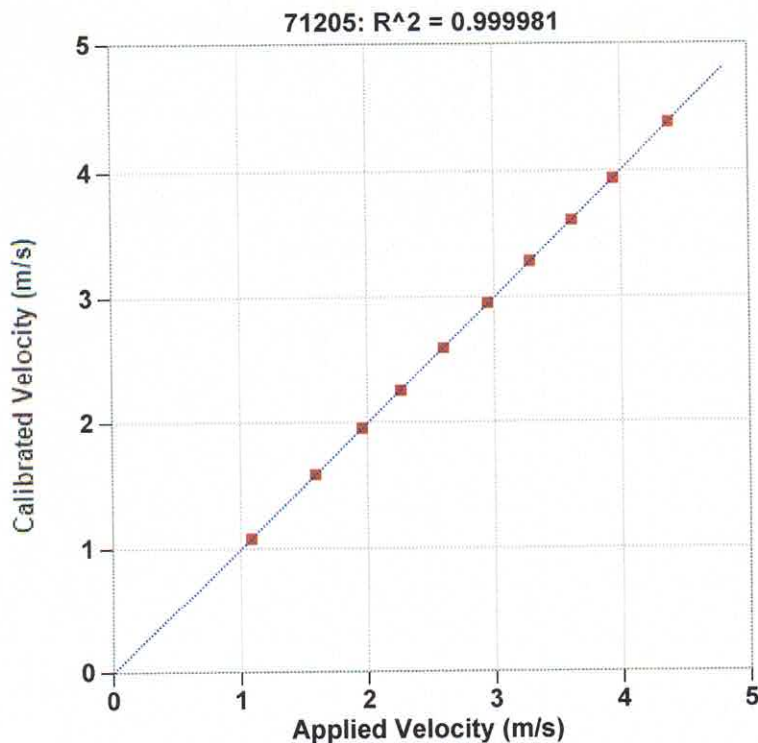

Reference Velocity	S/N 71205 Velocity
m/s	m/s
1.084	1.082
1.590	1.590
1.957	1.955
2.264	2.257
2.599	2.594
2.949	2.955
3.279	3.285
3.613	3.613
3.940	3.942
4.377	4.374
Maximum Acceleration: 959 g's	