

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K11956 Temperature: 23.0 °C
Model: KICHER PR Humidity: 28%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

440.9 mv/5000g
(88.2 μ v/g)
R²: 0.999969 [Chip programmed]

Ref Acc 1: 78268! Cal on: 11Jan2024
986 g's/volt
Ref Acc 2: 78270! Cal on: 11Jan2024
971 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 17Mar2025

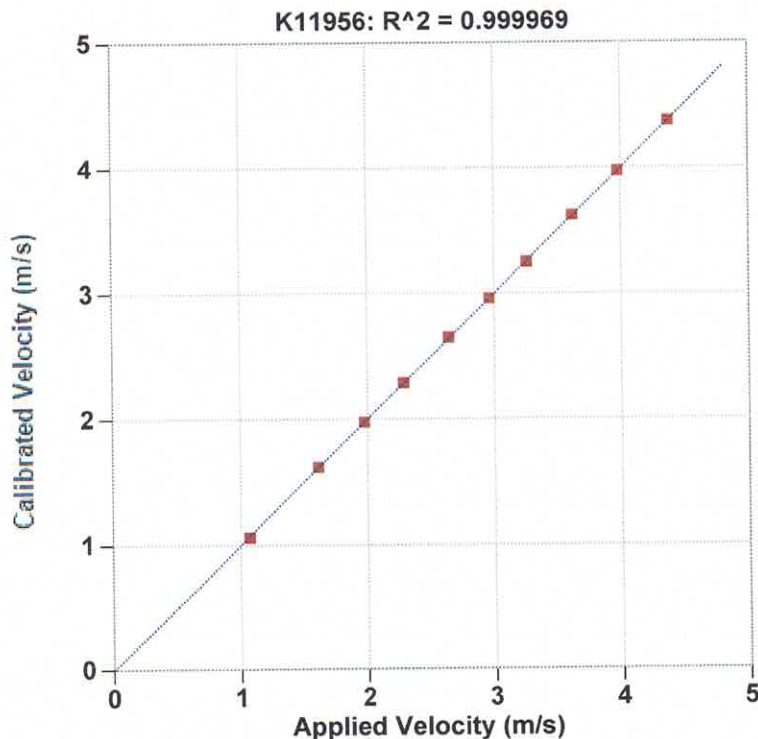

Reference Velocity	S/N K11956 Velocity
m/s	m/s
1.071	1.061
1.612	1.617
1.975	1.973
2.287	2.288
2.643	2.652
2.960	2.960
3.257	3.248
3.618	3.620
3.975	3.976
4.373	4.373

Maximum Acceleration: 963 g's