

Certificate of Calibration  
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K12608      Temperature: 23.1 °C  
Model: KICHER PR      Humidity: 28%  
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

406.4 mv/5000g  
(81.3 μv/g)  
R^2: 0.999926 [Chip programmed]

Ref Acc 1: 78268!      Cal on: 11Jan2024  
986 g's/volt  
Ref Acc 2: 78270!      Cal on: 11Jan2024  
971 g's/volt


Operator: William Johnson

  
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 17Mar2025

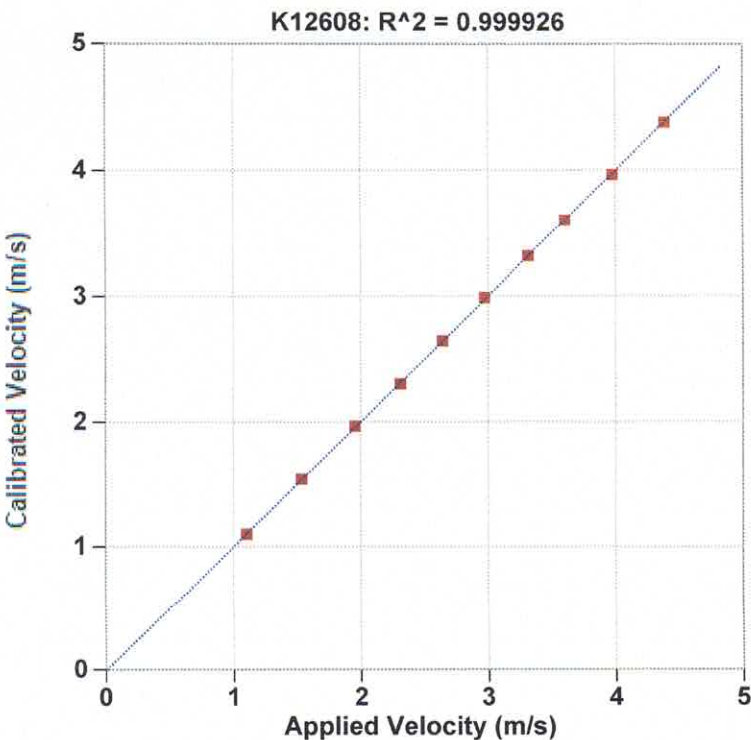

| Reference Velocity            | S/N K12608 Velocity |
|-------------------------------|---------------------|
| m/s                           | m/s                 |
| 1.103                         | 1.104               |
| 1.536                         | 1.542               |
| 1.954                         | 1.968               |
| 2.310                         | 2.307               |
| 2.643                         | 2.649               |
| 2.972                         | 2.988               |
| 3.314                         | 3.314               |
| 3.604                         | 3.601               |
| 3.978                         | 3.966               |
| 4.385                         | 4.378               |
| Maximum Acceleration: 964 g's |                     |