

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K12782 Temperature: 23.5 °C
Model: KICHER PR Humidity: 35%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

438.1 mv/5000g
(87.6 µv/g)
R²: 0.999965 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt


Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Operator: William Johnson


Signed

Calibration valid 2 years

From: 20Mar2025

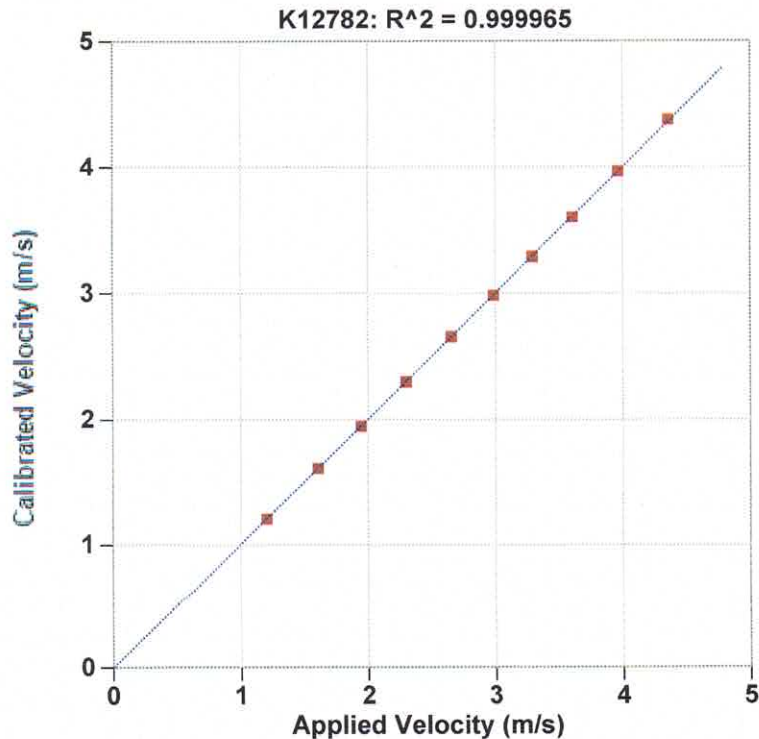

Reference Velocity	S/N K12782 Velocity
m/s	m/s
1.205	1.205
1.607	1.610
1.945	1.943
2.298	2.298
2.654	2.655
2.985	2.983
3.293	3.285
3.607	3.600
3.964	3.962
4.355	4.370
Maximum Acceleration: 942 g's	