

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K14530 Temperature: 22.6 °C
Model: KICHER PR Humidity: 26%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

402.4 mv/5000g
(80.5 μ v/g)
R²: 0.999959 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt

Operator: William Johnson

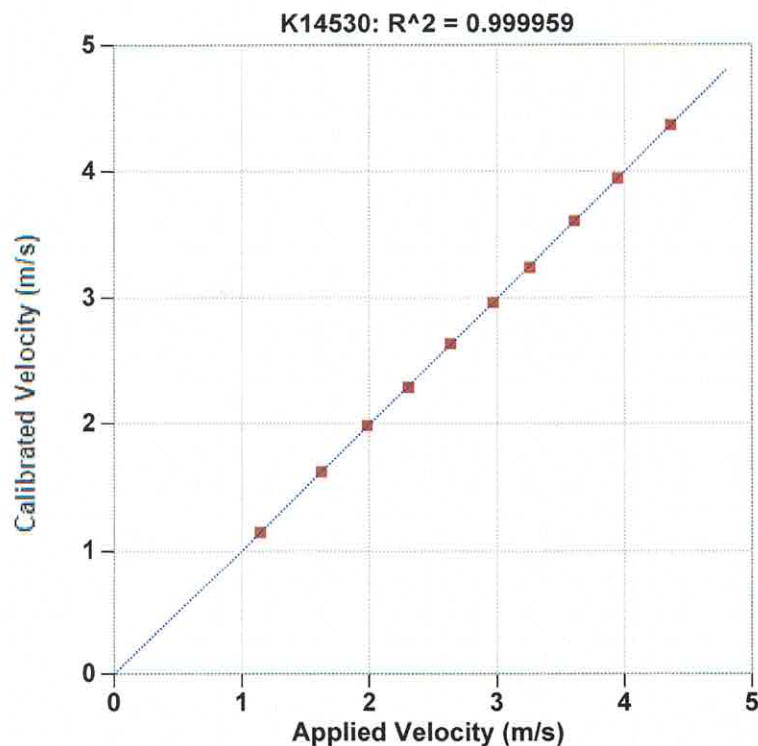

Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

MAR 24 2025

From: _____



Reference Velocity	S/N K14530 Velocity
m/s	m/s
1.143	1.145
1.621	1.622
1.981	1.988
2.306	2.295
2.635	2.638
2.969	2.966
3.259	3.246
3.607	3.611
3.946	3.951
4.363	4.366

Maximum Acceleration: 963 g's