

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K14538 Temperature: 23.3 °C
Model: KICHER PR Humidity: 28%
Calibrated on: Channel 4 on 8G 5161 LE

Ref Acc 1: 78270! Cal on: 11Jan2024
971 g's/volt
Ref Acc 2: 78268! Cal on: 11Jan2024
986 g's/volt

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR


385.2 mv/5000g
(77.0 μv/g)
R^2: 0.999956 [Chip programmed]

Operator: William Johnson


Signed

Calibration valid 2 years

From: MAR 24 2025

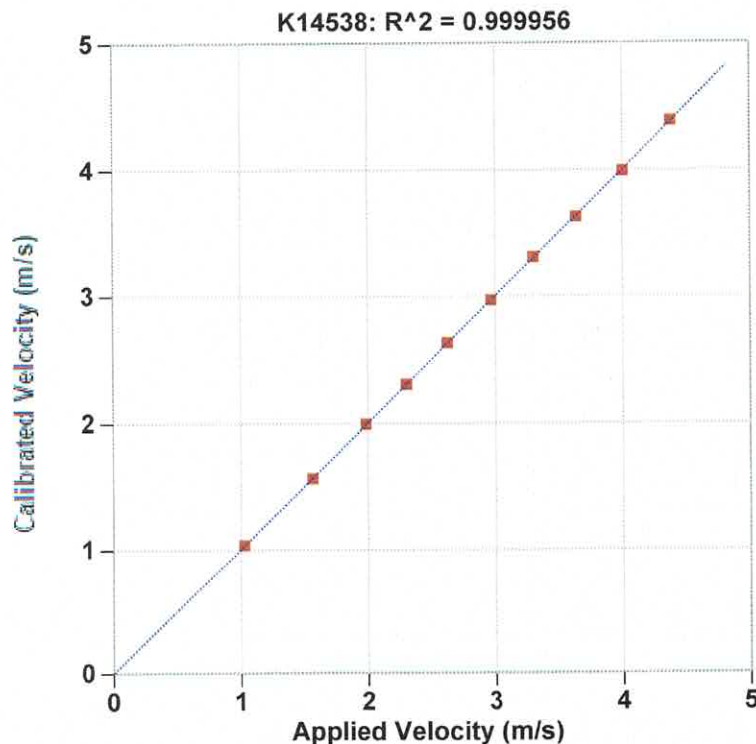

Reference Velocity	S/N K14538 Velocity
m/s	m/s
1.026	1.033
1.562	1.561
1.981	1.990
2.300	2.304
2.623	2.629
2.966	2.962
3.299	3.305
3.635	3.627
4.001	3.990
4.378	4.383

Maximum Acceleration: 955 g's