



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: W776


PDI Gage Factor: 94.4

Mean Linear Correlation Coefficient: 0.999825

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1583.3	-4.799	508.3	1.721
-1141.7	-3.408	816.7	2.660
-775.0	-2.258	1133.3	3.612
-483.3	-1.362	1450.0	4.544
-183.3	-0.432	1766.7	5.475
191.7	0.753	2000.0	6.142

Calibration Curve

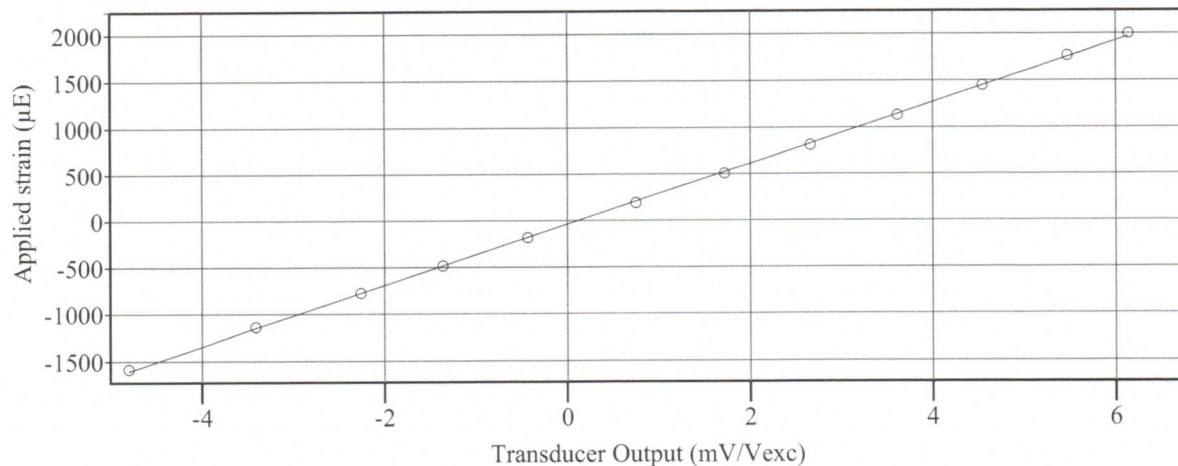

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: W776

Calibration Date: 3/20/2025 1:35:31 PM

