



Pile Dynamics, Inc.


Pile Dynamics, Inc.

Transducer 104W

Strain ($\mu\epsilon$)

PDA Cal Factor (5.0 V)

110.9 $\mu\epsilon/V$

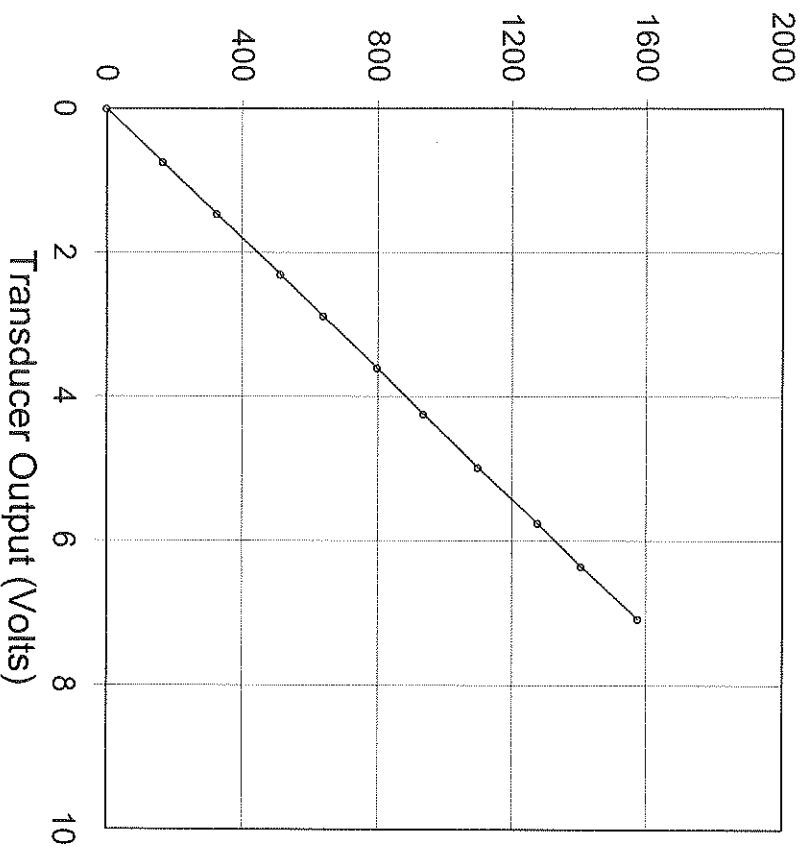

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
169	0.74
325	1.46
512	2.30
637	2.88
799	3.60
937	4.24
1099	4.98
1279	5.75
1408	6.35
1577	7.08

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Shunt (60.4 K Ω) 2.5 V
General Factor 385.2 $\mu\epsilon/mV/V$
Calibrated by: George Powell
Calibrated on: 22-Aug-2007