


Pile Dynamics, Inc. Transducer 105W

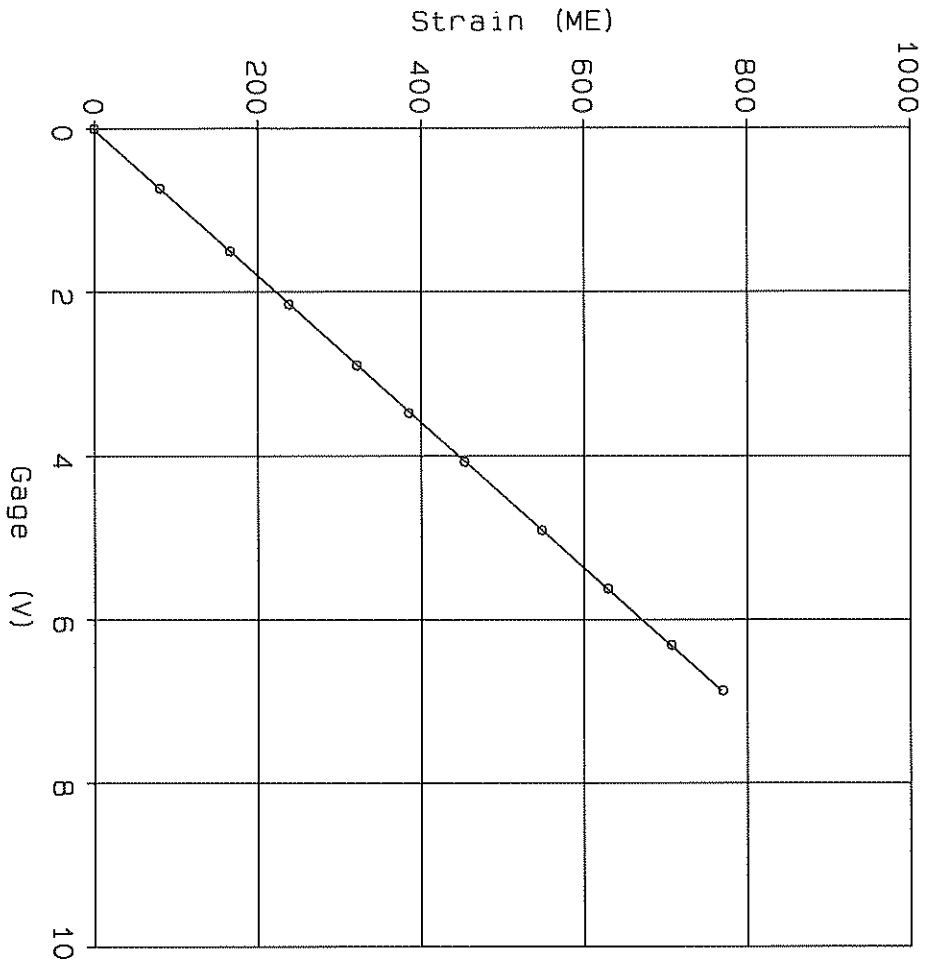

PDA Cal Factor = 112.1 ME/V
Shunt (60.4K) = 5.0 V

General Factor = 389.3 ME/mV/V
Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
81	.73
166	1.50
239	2.15
321	2.90
386	3.48
453	4.08
548	4.92
629	5.63
707	6.32
771	6.88

Calibrated by: Jim Stambold
Calibrated on: 15-May-95