




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer

108W

Strain ($\mu\epsilon$)

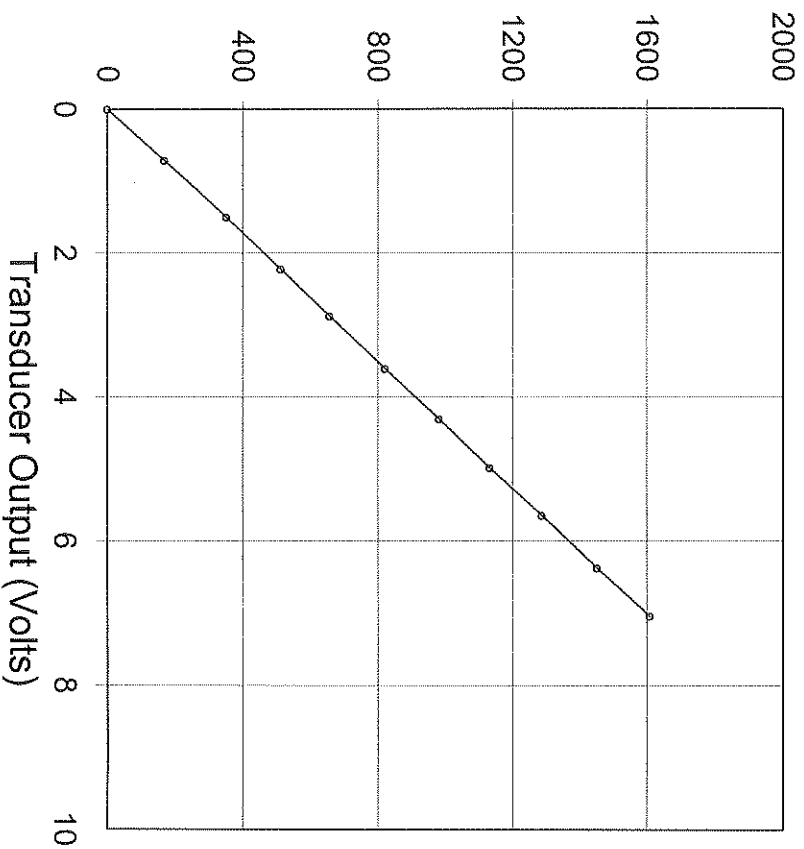

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

113.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
171	0.71
351	1.50
512	2.22
658	2.87
822	3.60
981	4.30
1133	4.98
1288	5.64
1454	6.37
1609	7.04

Shunt (60.4 K Ω)

2.5 V
395.0 $\mu\epsilon/mV/V$

Calibrated by:

Greg P. [Signature]

Calibrated on:

22-Aug-2007