


Pile Dynamics Inc Transducer 110M

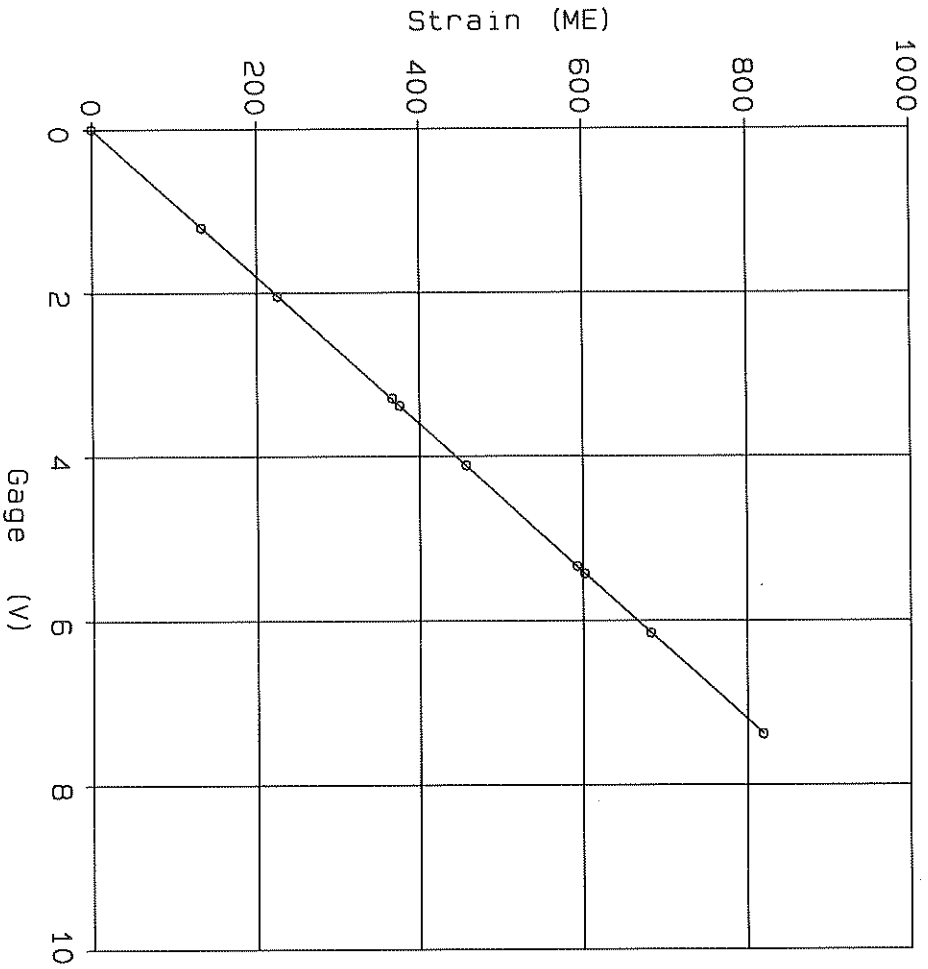

PDA Cal Factor = 111.1 ME/V
Shunt (60.4K) = 5.0 V

General Factor = 385.7 ME/mV/V
Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
134	1.21
133	1.21
227	2.04
368	3.30
377	3.39
457	4.11
594	5.33
603	5.42
683	6.16
819	7.38

Calibrated by: *J. S. [Signature]*
Calibrated on: 07-Sep-99