


Pile Dynamics, Inc. Transducer 110W

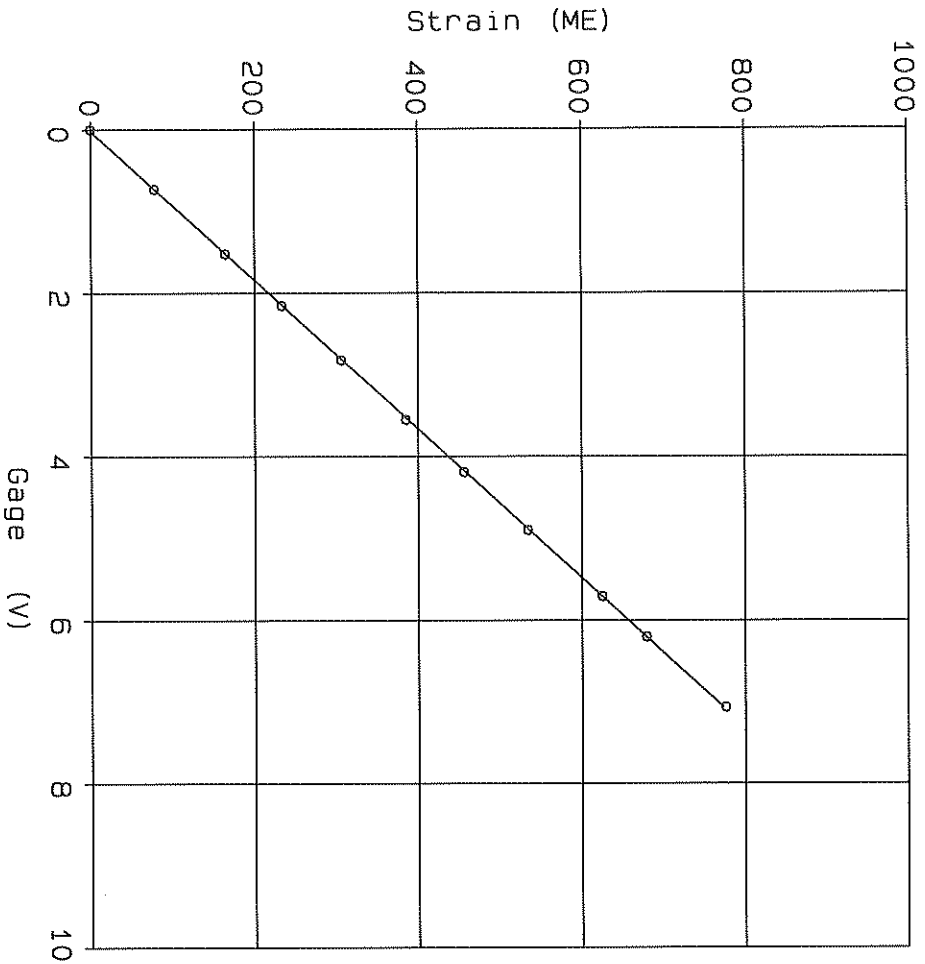

PDA Cal Factor = 109.9 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 381.7 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
78	.73
164	1.53
233	2.16
306	2.83
385	3.55
456	4.20
535	4.90
626	5.71
680	6.20
777	7.07

Calibrated by: *Jim Douthett*
 Calibrated on: 15-May-95