


Pile Dynamics, Inc. Transducer 115W

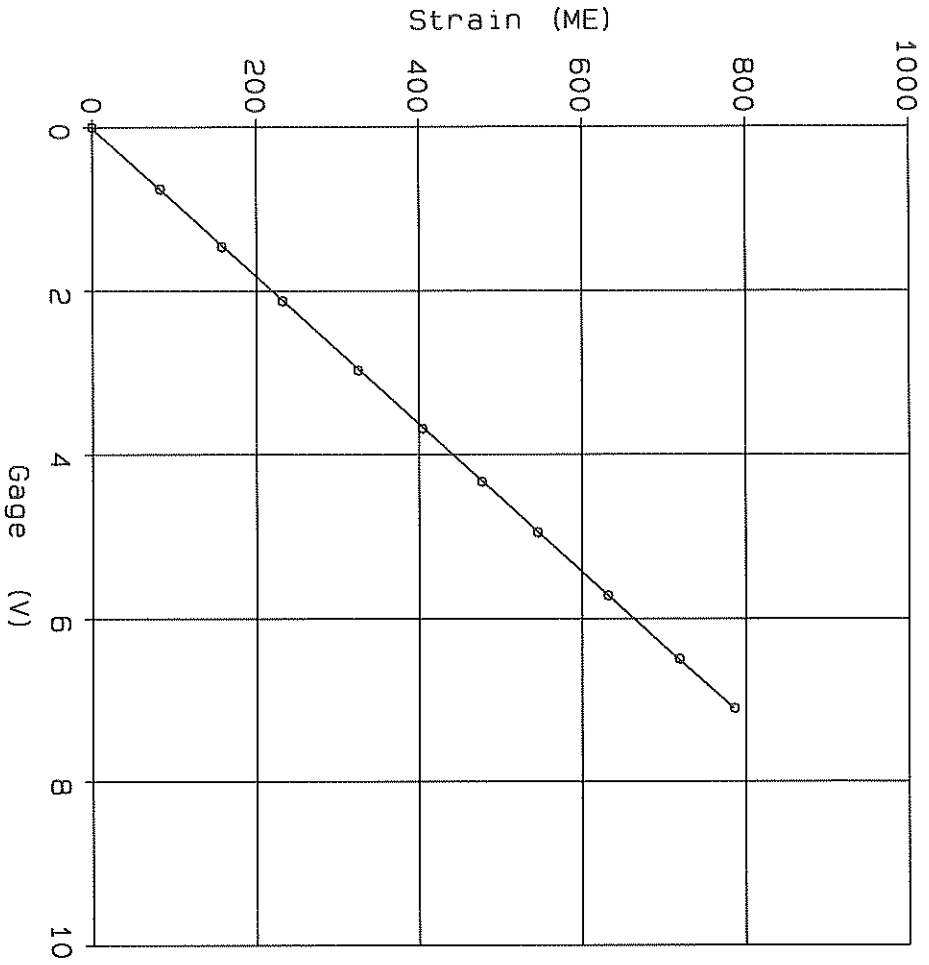

PDA Cal Factor = 110.9 ME/V
 Shunt (60.4K0) = 5.0 V
 General Factor = 385.2 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
83	.77
159	1.46
232	2.13
326	2.97
405	3.69
477	4.34
546	4.95
633	5.72
719	6.49
787	7.11

Calibrated by:
 Calibrated on: 28-Jul-95