


PILE DYNAMICS, INC.

GAGE NO. 453D

08-AUG-87

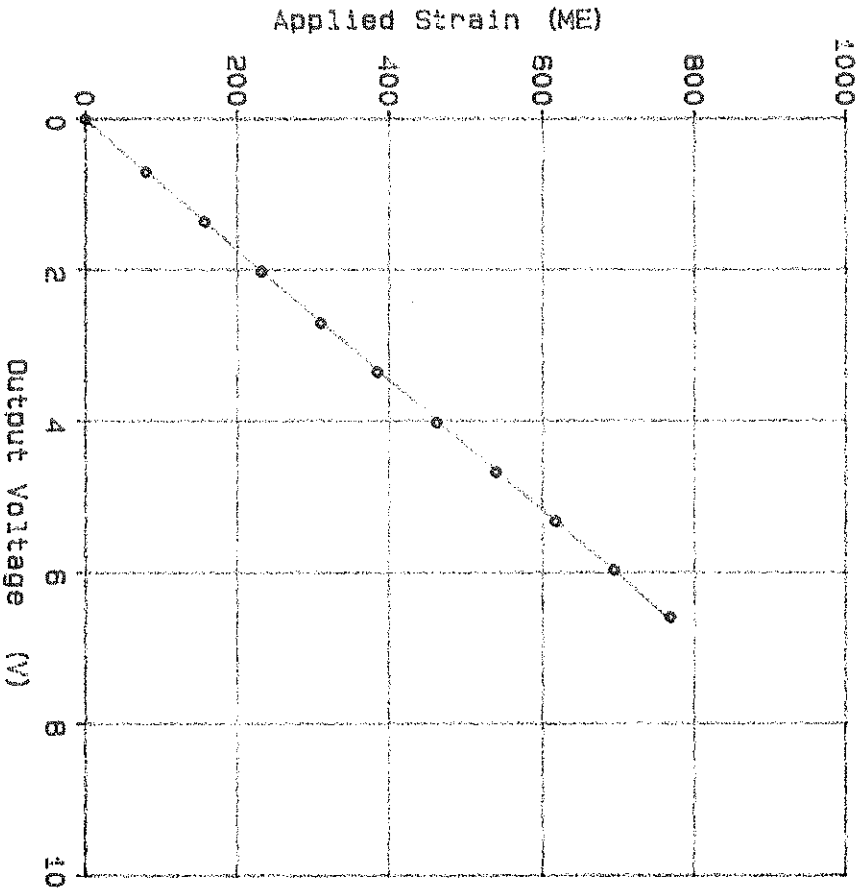

Gage Calibration Factor = 116.4 ME/V
 Gage Ref. Shunt (60.4KΩ) = 5.0 VOLTS
 Offset = -2.5

No.	Applied Strain ME	Gage Voltage V
1	.0	.00
2	80.0	.70
3	156.1	1.37
4	232.4	2.03
5	310.1	2.71
6	384.8	3.35
7	462.6	4.02
8	539.2	4.67
9	616.3	5.33
10	693.1	5.96
11	768.3	6.60