




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer 155W

Strain ($\mu\epsilon$)

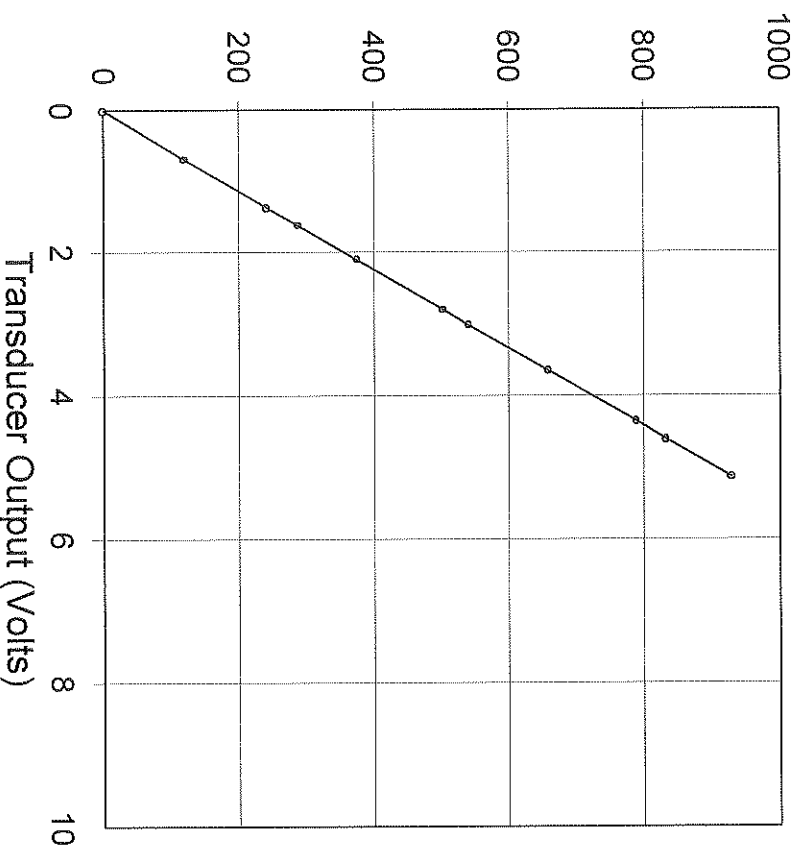

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor

182.3 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
120	0.69
241	1.37
288	1.63
374	2.10
503	2.80
539	3.01
658	3.64
789	4.34
833	4.60
929	5.12

Shunt (60.4 K Ω)

5.0 V

General Factor

632.9 $\mu\epsilon/mV/V$

Calibrated by: Frank Rhubert

Calibrated on:

12-Nov-2004