




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer

160W

Strain ($\mu\epsilon$)

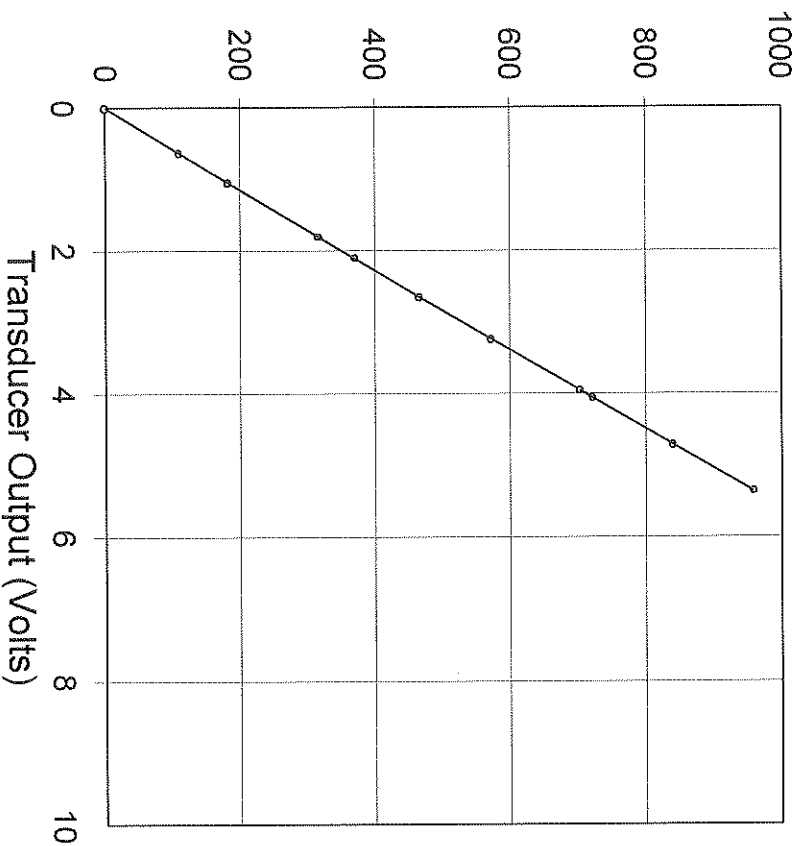

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor

179.4 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
109	0.63
182	1.05
316	1.80
369	2.10
466	2.64
571	3.23
722	4.05
703	3.94
840	4.71
959	5.35

Shunt (60.4 K Ω) 5.0 V
General Factor 623.0 $\mu\epsilon/mV/V$

Calibrated by: Tim Rube
Calibrated on: 11-Nov-2004