


Pile Dynamics, Inc. Transducer 163W

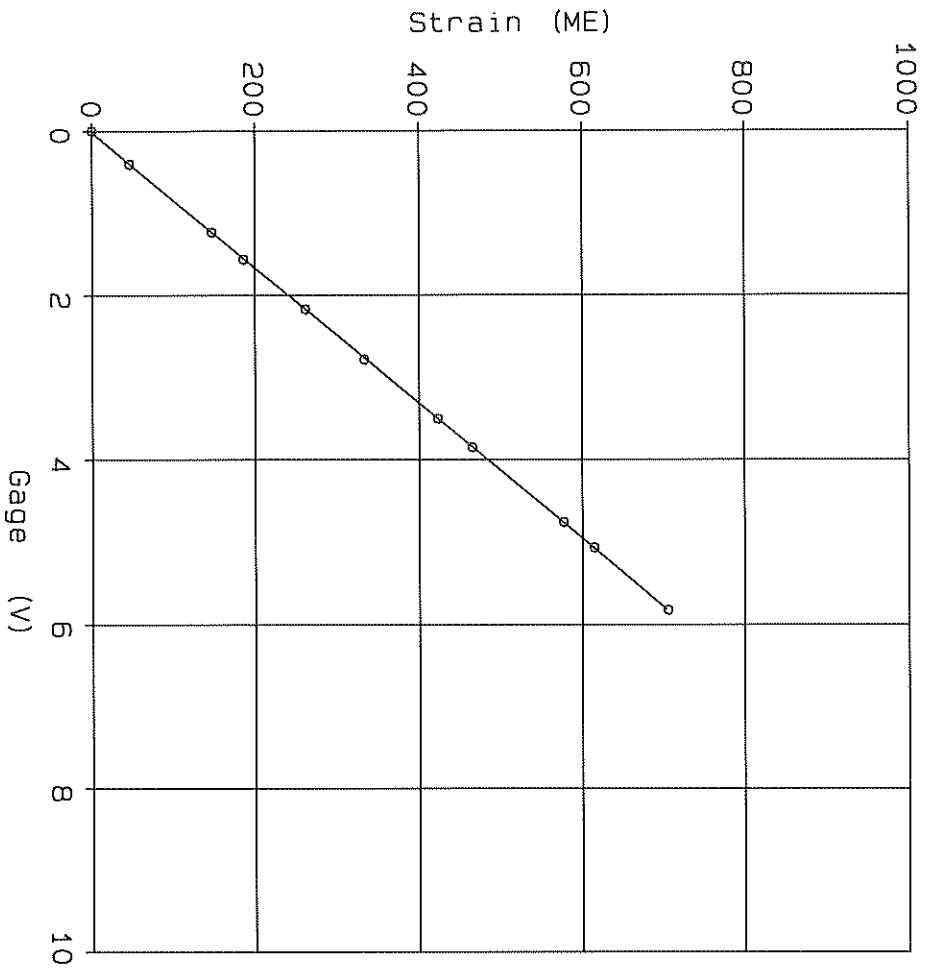

PDA Cal Factor = 121.6 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 422.1 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
47	.41
147	1.23
187	1.57
261	2.18
333	2.78
423	3.51
465	3.86
578	4.77
615	5.07
707	5.83

Calibrated by: *J. S. Suber*
 Calibrated on: 31-May-96