


Pile Dynamics, Inc. Transducer 164W

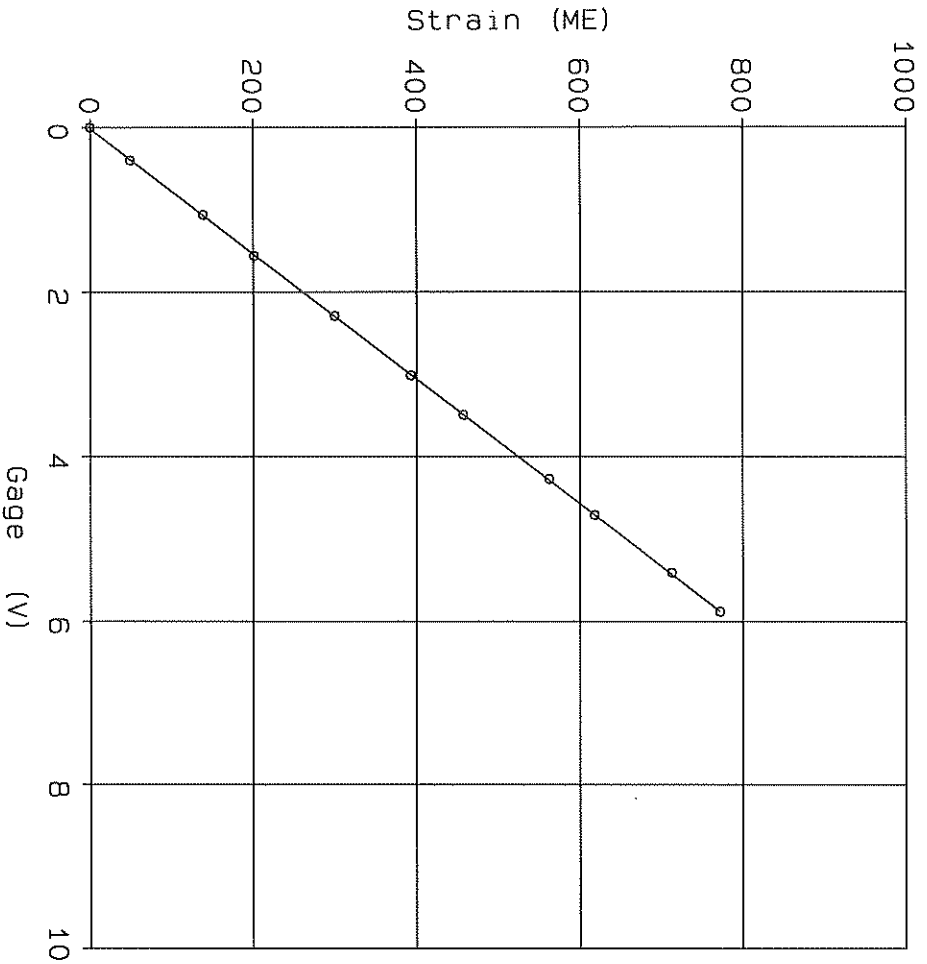

PDA Cal Factor = 131.8 ME/V
Shunt (60.4K0) = 5.0 V

General Factor = 457.8 ME/mv/V
Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
49	.40
138	1.06
201	1.57
300	2.30
394	3.02
458	3.49
562	4.28
619	4.72
713	5.42
772	5.88

Calibrated by: *[Signature]*
Calibrated on: 31-May-96