Pile Dynamics, Inc.
Transducer 169I

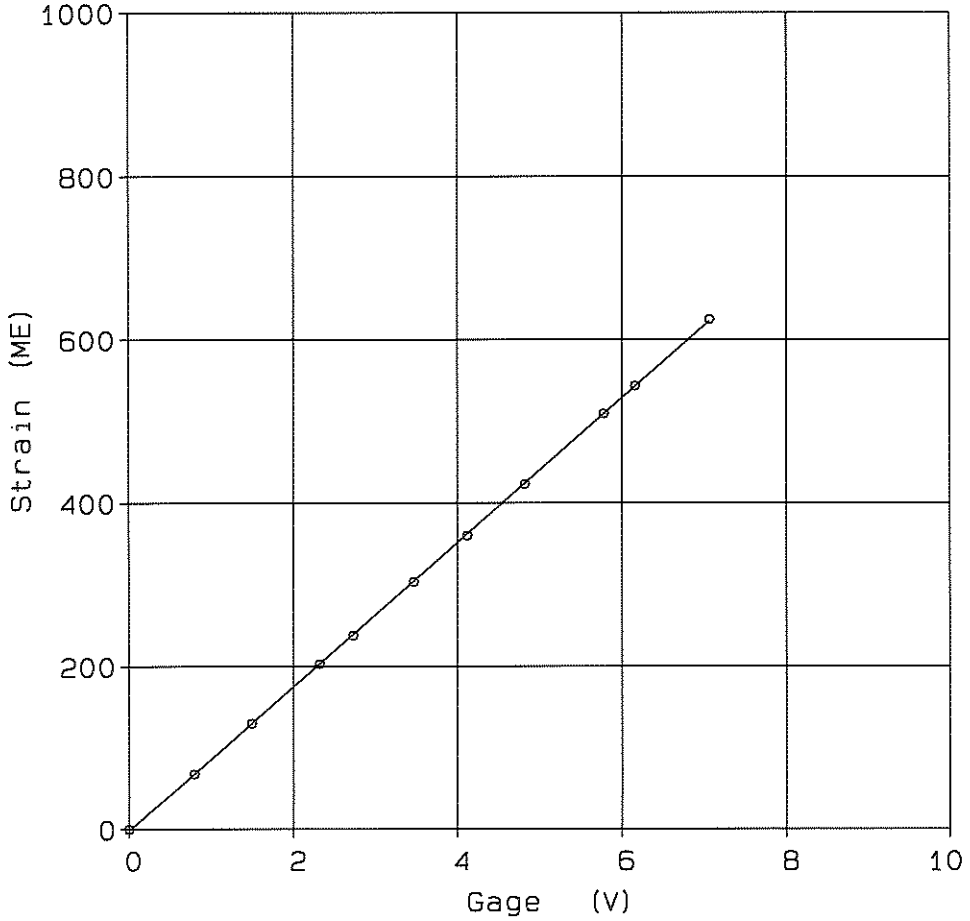

PDA Cal Factor	=	88.4 ME/V
Shunt (60.4KO)	=	5.0 V
General Factor	=	307.0 ME/mV/V

Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
69	.79
130	1.50
203	2.32
239	2.74
304	3.47
361	4.12
424	4.82
509	5.78
543	6.16
625	7.07

Calibrated by: Jim Deutschendorff

Calibrated on: 24-Jan-95

Strain Transducer Calibration System - Version 1994-2